

File ..\DATA\2020\20200422\935\BIZ2020-421-SCH1-.D Tgt Mass (CHM):

Injection Date : 22 Apr 20 12:34 pm +0800 Seq. Line : 47

Sample Name : BIZ2020-421-SCH1 Location : PL-B-01

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.5 ul

Acq. Method : D:\Chem32\1\data\2020\20200422\935\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200422\935\1-POS-3MIN.M

Catalog No : HY-112445 Batch# 63240

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

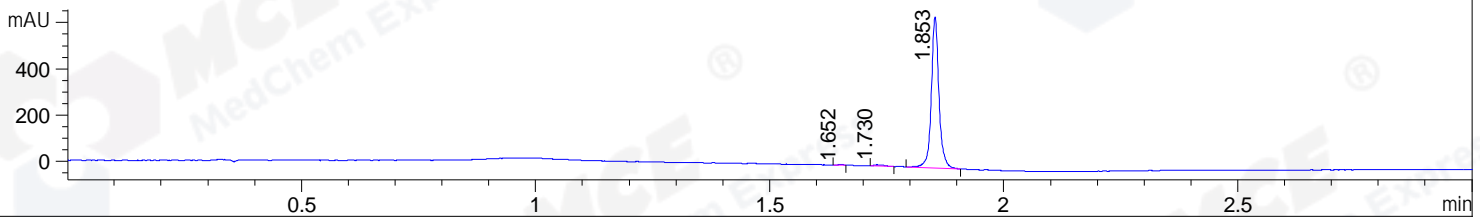


DAD1 C, Sig=254,4 Ref=off

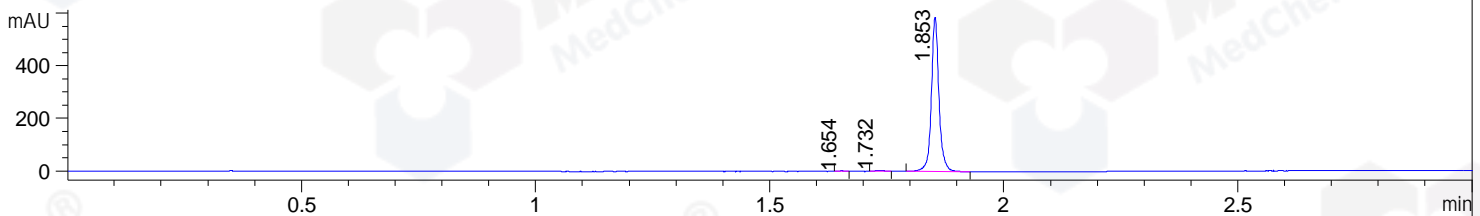

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

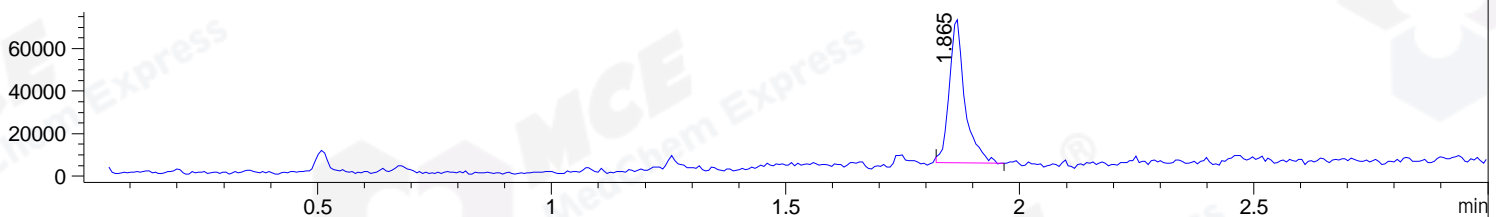

Ion 787, MSD1 787, Target Mass 786 +H Positive, EIC=786.7:787.7

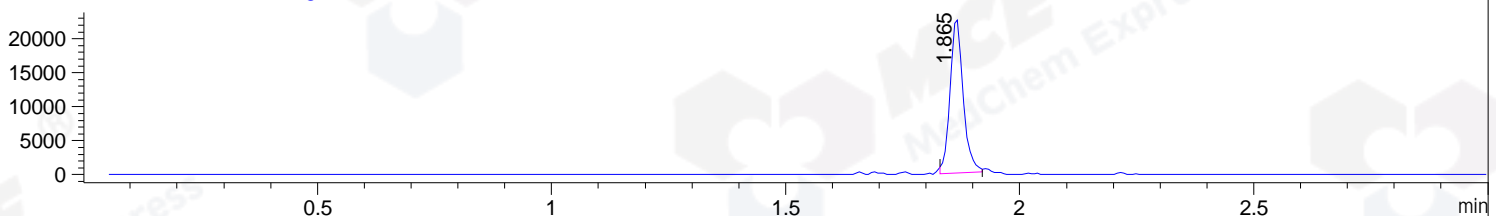

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.01	1.89	2.59	0.25	ND
1.73	0.02	9.21	6.23	1.23	ND
1.85	0.02	739.77	655.24	98.52	787

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.01	1.88	2.31	0.28	ND
1.73	0.02	5.17	3.63	0.77	ND
1.85	0.02	661.32	587.45	98.94	787

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.86	0.03	157843.47	68776.85	100.00	787

Ret. Time: 1.86

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

