

File ..1\DATA\2019\20190405\562\BIZ2019-403-WYQ7.D Tgt Mass (CHM):

Injection Date : 5 Apr 19 11:09 am +0800 Seq. Line : 29

Sample Name : BIZ2019-403-WYQ7 Location : P2-E-02

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190405\562\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190405\562\1-POS-3MIN-1.M

Catalog No : HY-112701 Batch#39725

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

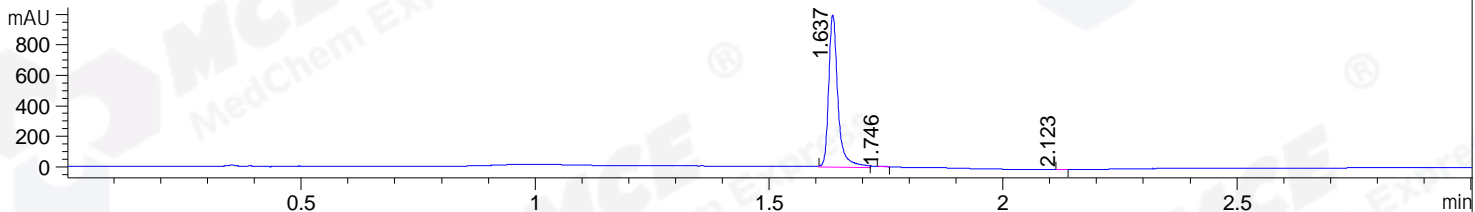


DAD1 C, Sig=254,4 Ref=off

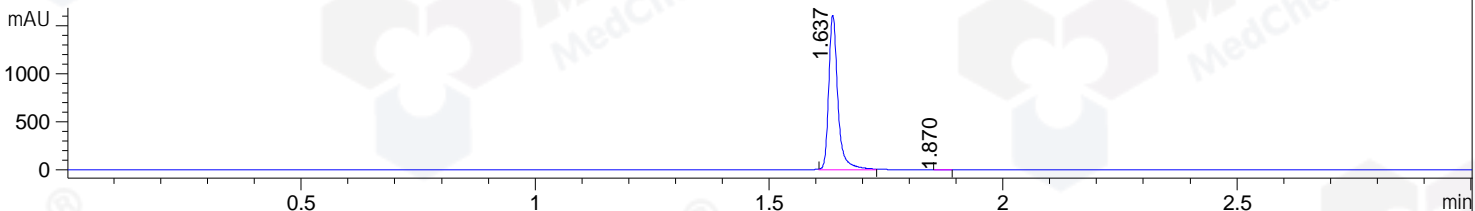

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

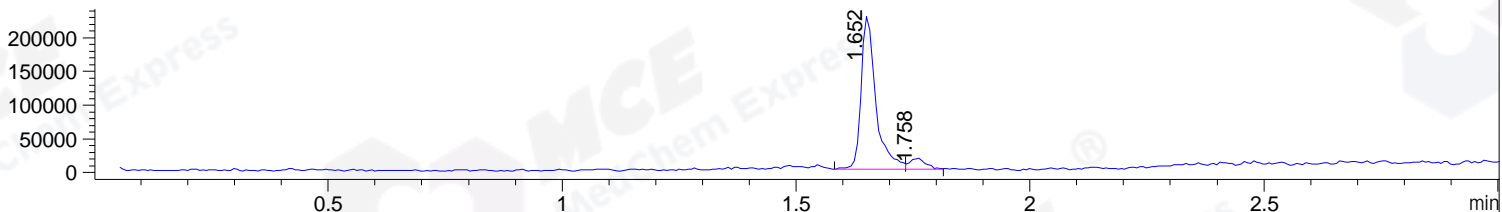

Ion 505.1, MSD1 505.1, Target Mass 504.1 +H Positive, EIC=504.8:505.8

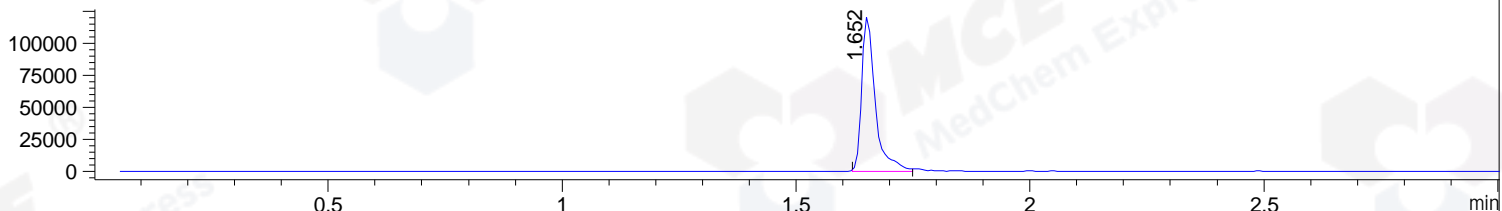

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.64	0.02	1376.98	969.75	99.82	505
1.75	0.01	1.61	2.01	0.12	505
2.12	0.01	0.86	0.99	0.06	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.64	0.02	2203.41	1562.47	99.89	505
1.87	0.02	2.35	2.04	0.11	ND


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.03	501393.72	227827.69	92.82	505
1.76	0.04	38781.74	15570.81	7.18	279

Ret. Time: 1.65

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

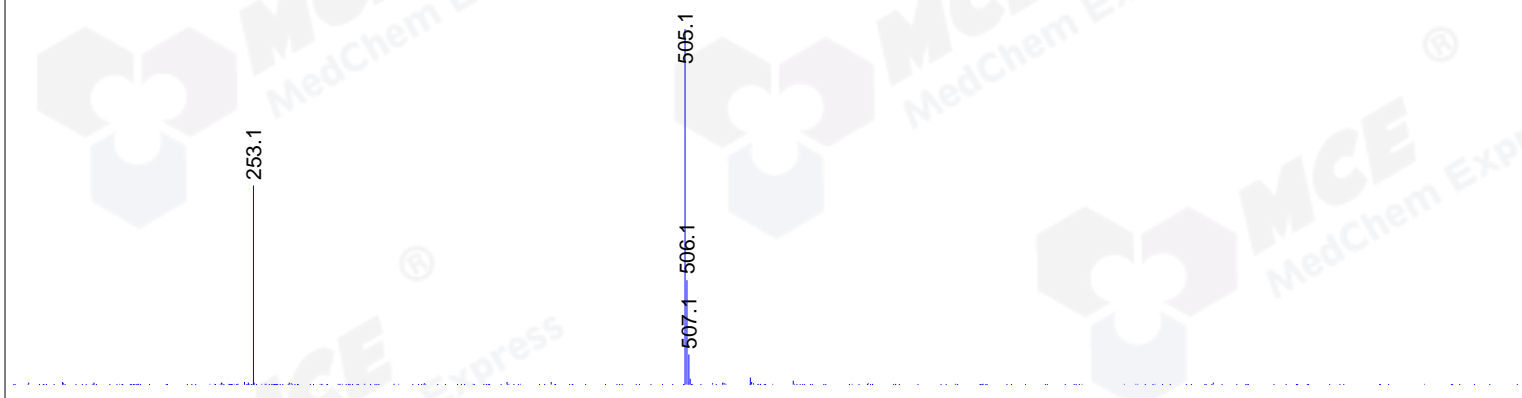

Ret. Time: 1.76

ES-API Positive

