

File ..\DATA\2020\20200403\911\BIZ2020-402-CXL7.D Tgt Mass (CHM):

Injection Date : 3 Apr 20 12:29 pm +0800 Seq. Line : 46

Sample Name : BIZ2020-402-CXL7 Location : PL-A-02

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.7 ul

Acq. Method : D:\Chem32\1\data\2020\20200403\911\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200403\911\1-POS-3MIN.M

Catalog No : HY-112852 Batch# 62232

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

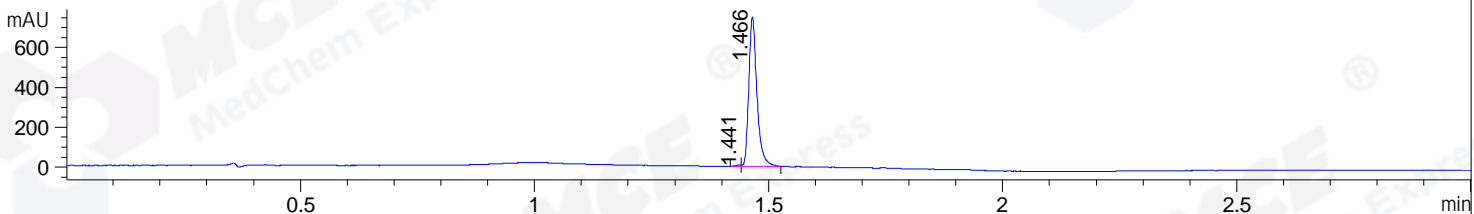


DAD1 C, Sig=254,4 Ref=off

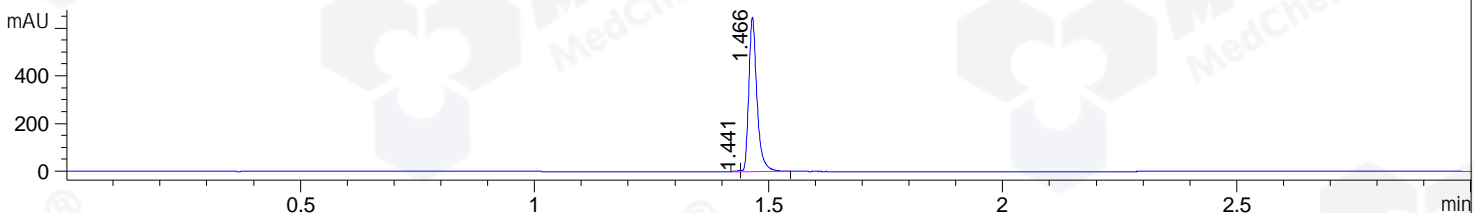

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

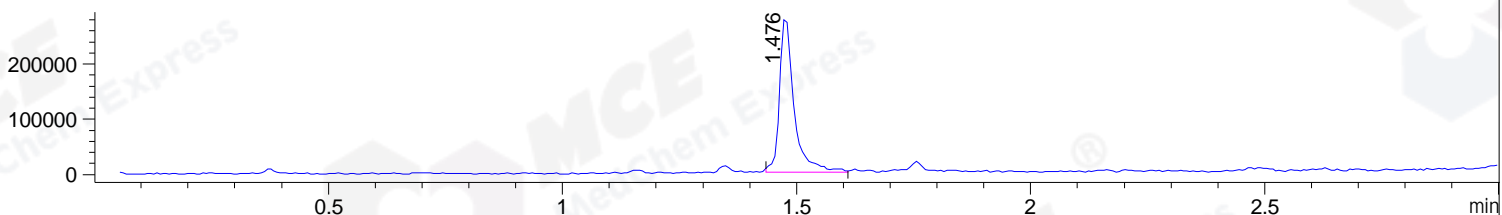

Ion 610, MSD1 610, Target Mass 609 +H Positive, EIC=609.7:610.7

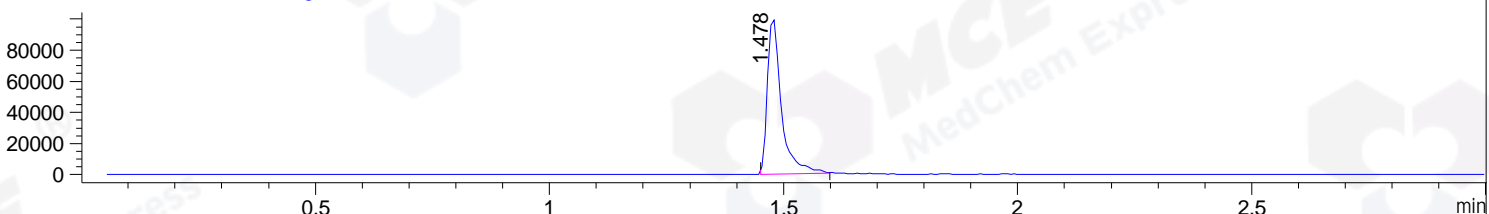

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.44	0.01	4.38	5.17	0.48	491
1.47	0.02	904.84	748.92	99.52	306

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.44	0.01	2.59	3.58	0.33	491
1.47	0.02	784.02	647.70	99.67	306

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.03	603888.63	284264.09	100.00	306

Ret. Time: 1.48

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

