

File ..1\DATA\2019\20190619\597\BIZ2019-618-WYQ1.D Tgt Mass (CHM):

Injection Date : 19 Jun 19 11:00 am +0800 Seq. Line : 10

Sample Name : BIZ2019-618-WYQ1 Location : P2-A-03

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190619\597\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190619\597\1-POS-3MIN.M

Catalog No : HY-113219 Batch#42427

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

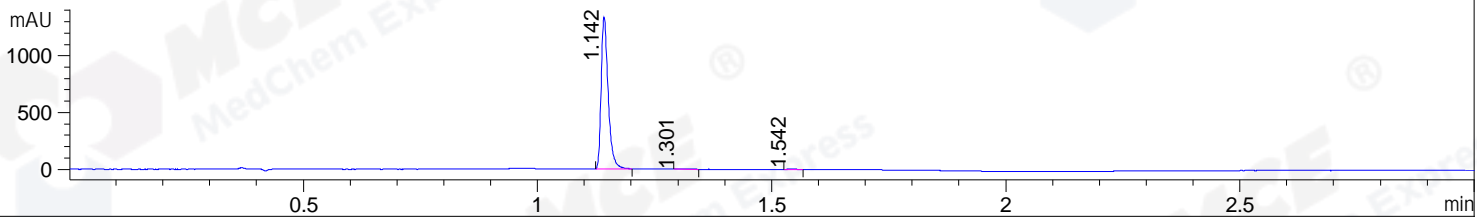


DAD1 C, Sig=254,4 Ref=off

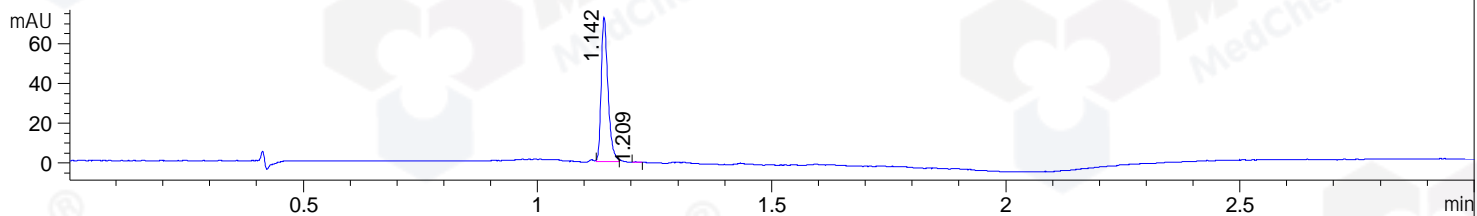

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

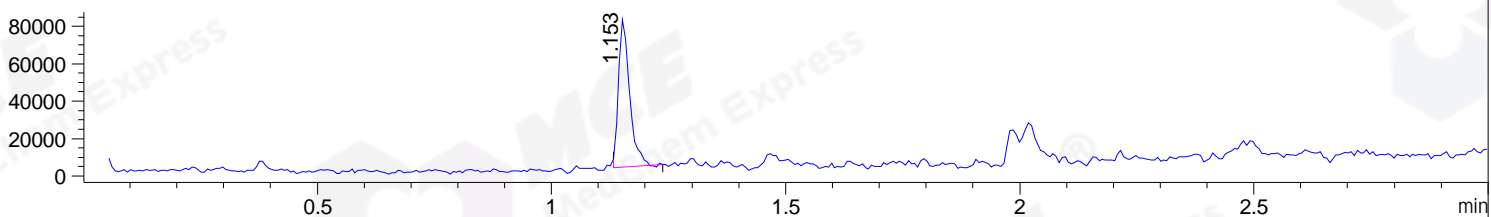

Ion 183, MSD1 183, Target Mass 182 +H Positive, EIC=182.7:183.7

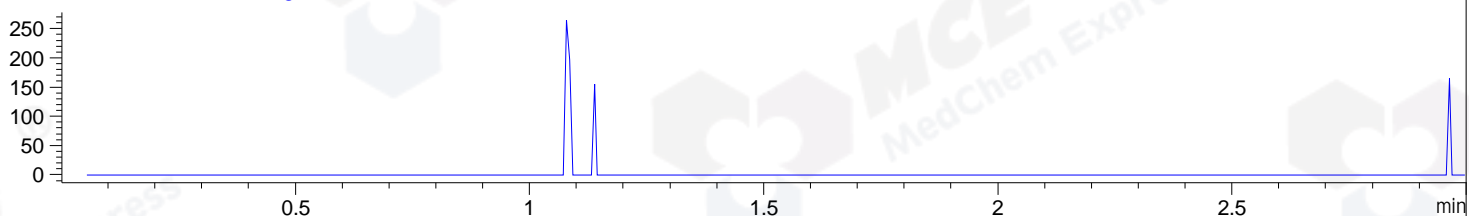

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.14	0.02	1401.69	1341.71	99.19	205
1.30	0.02	4.35	3.88	0.31	ND
1.54	0.01	7.04	7.44	0.50	ND

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.14	0.02	73.20	72.55	99.72	205
1.21	0.01	0.20	0.26	0.28	ND

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.03	130458.53	79540.51	100.00	205

Ret. Time: 1.15

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

