


SAMPLE INFORMATION

Sample Name:		Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	6	Acq. Method Set:	
Injection #:	1	Processing Method:	Quality Guarantee System
Injection Volume:	10.00 ul	Channel Name:	220.0nm
Run Time:	100.0 Minutes	Proc. Chnl. Descr.:	PDA 220.0 nm
Catalog No:	HY-113573 Batch#40870		
Date Acquired:	2018-5-25 13:07:14 CST		
Date Processed:	2019-5-8 13:20:10 CST		

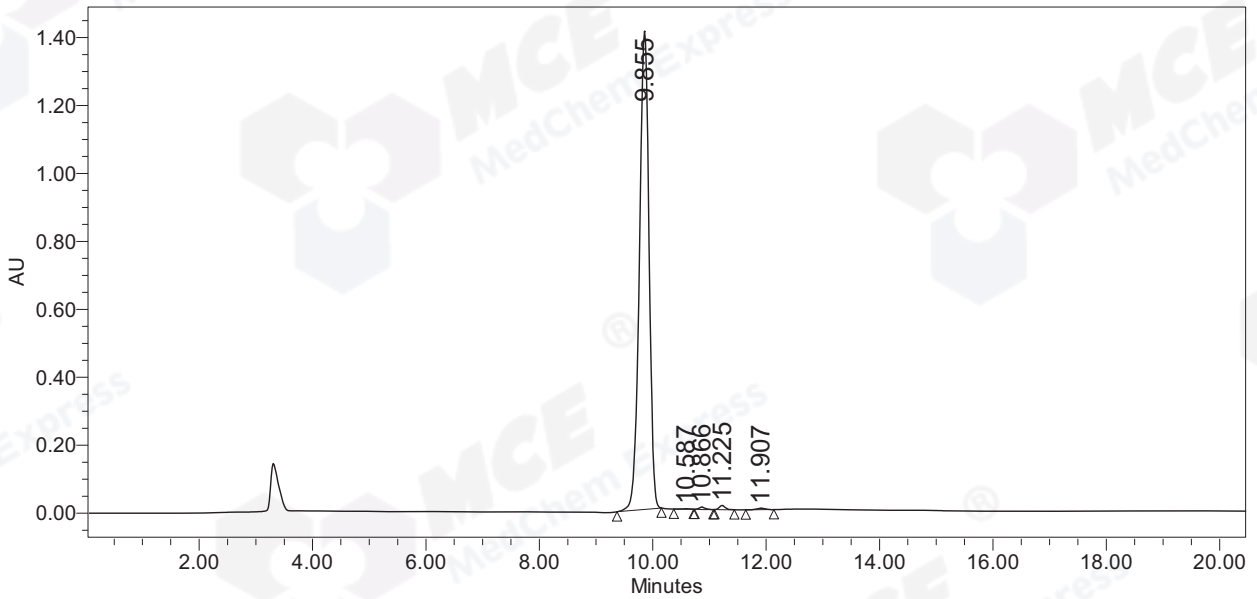

	RT	Area	% Area	Height
1	9.855	16716950	98.88	1406996
2	10.587	15846	0.09	1720
3	10.866	48133	0.28	6750
4	11.225	85400	0.51	12226
5	11.907	39950	0.24	4234