

File ..1\DATA\2020\20200422\935\BIZ2020-420-WMX8.D Tgt Mass (CHM):

Injection Date : 22 Apr 20 4:11 pm +0800 Seq. Line : 95

Sample Name : BIZ2020-420-WMX8 Location : PL-B-05

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200422\935\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200422\935\1-POS-3MIN.M

Catalog No : HY-114116

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

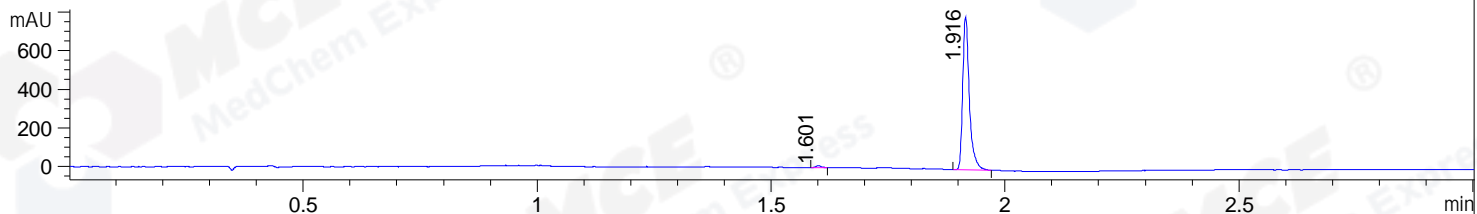


DAD1 C, Sig=254,4 Ref=off

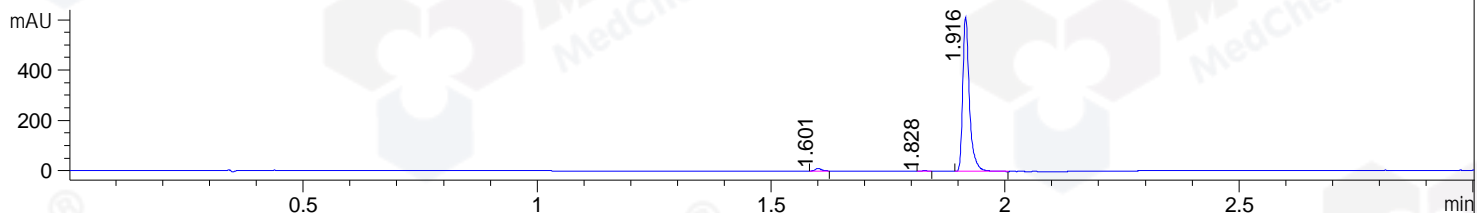

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

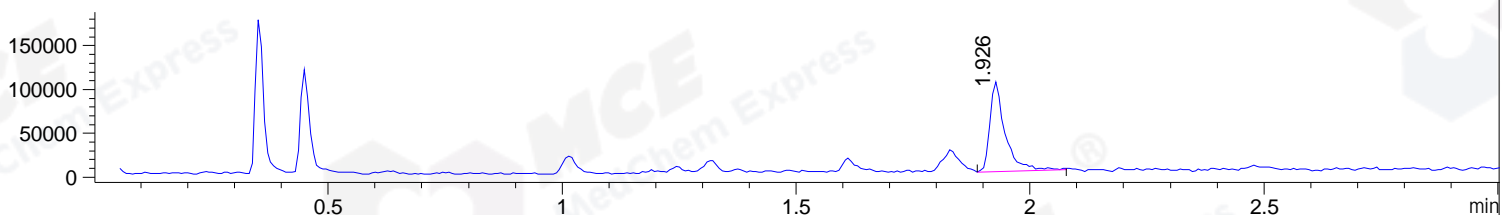

Ion 524, MSD1 524, Target Mass 523 +H Positive, EIC=523.7:524.7

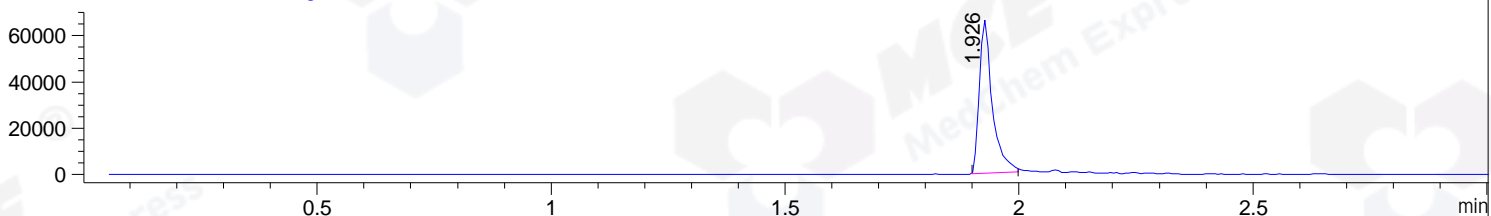

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.60	0.01	6.94	9.19	0.88	130
1.92	0.02	779.81	793.05	99.12	524

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.60	0.01	8.42	9.76	1.36	130
1.83	0.01	1.19	1.47	0.19	250
1.92	0.02	608.21	614.02	98.44	524

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.93	0.03	231230.13	102543.31	100.00	524

Ret. Time: 1.93

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

