

File ..\DATA\2019\20190410\559\BIZ2019-409-WYQ26.D Tgt Mass (CHM):

Injection Date : 10 Apr 19 3:20 pm +0800 Seq. Line : 79

Sample Name : BIZ2019-409-WYQ26 Location : PL-A-05

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190410\559\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190410\559\1-POS-3MIN-1.M

Catalog No : HY-114403 Batch#39975

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

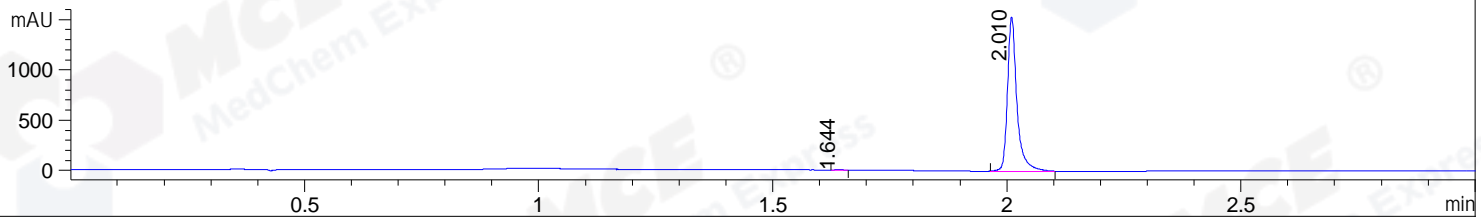


DAD1 C, Sig=254,4 Ref=off

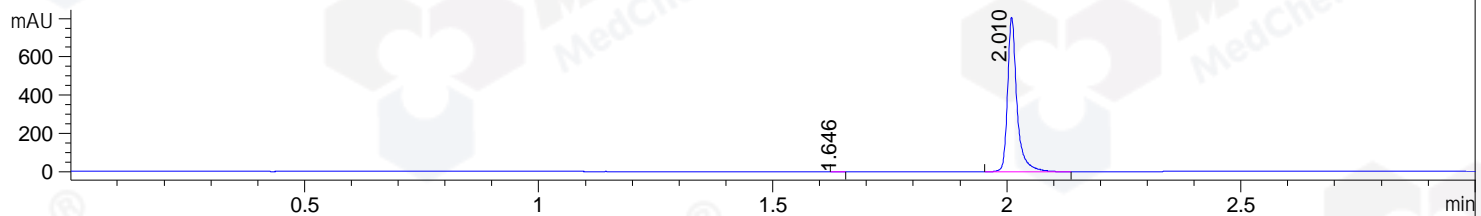

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

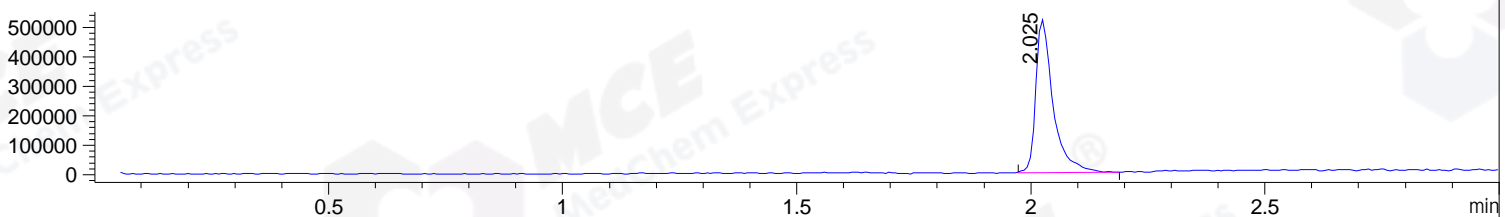

Ion 449.1, MSD1 449.1, Target Mass 448.1 +H Positive, EIC=448.8:449.8

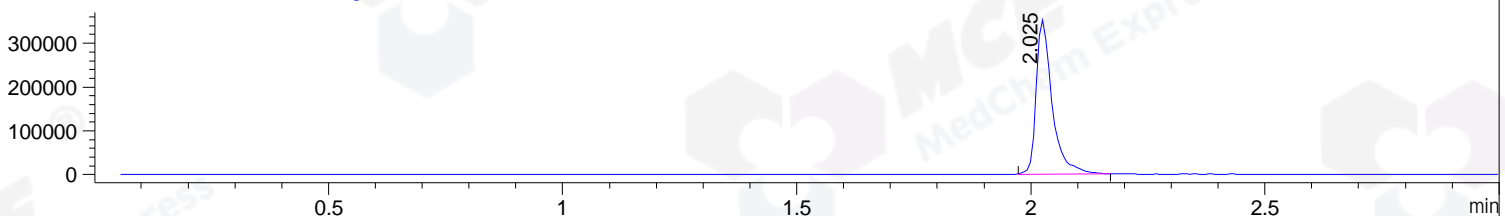

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.64	0.02	1.72	1.38	0.08	ND
2.01	0.02	2162.99	1534.82	99.92	449

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.02	0.48	0.36	0.04	ND
2.01	0.02	1142.65	809.50	99.96	449

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.02	0.04	1341413.25	519832.69	100.00	449

Ret. Time: 2.02

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

