

File ..\DATA\2019\20190510\570\BIZ2019-509-WYQ15.D Tgt Mass (CHM):

Injection Date : 10 May 19 1:53 pm +0800 Seq. Line : 36

Sample Name : BIZ2019-509-WYQ15 Location : P2-A-02

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190510\570\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190510\570\1-POS-3MIN.M

Catalog No : HY-114758 Batch#41060

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-322

Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

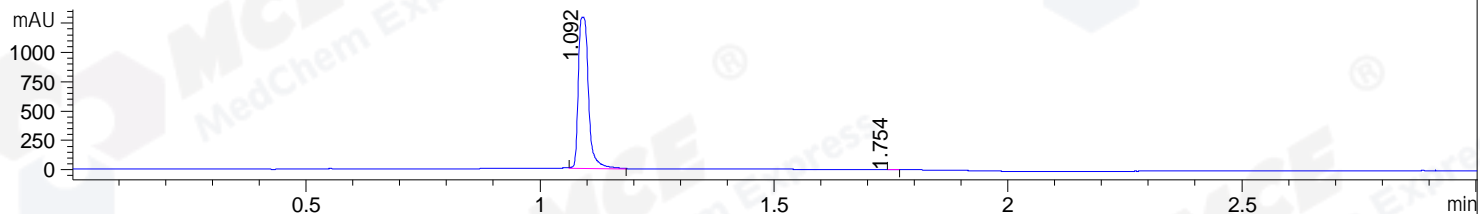


DAD1 C, Sig=254,4 Ref=off

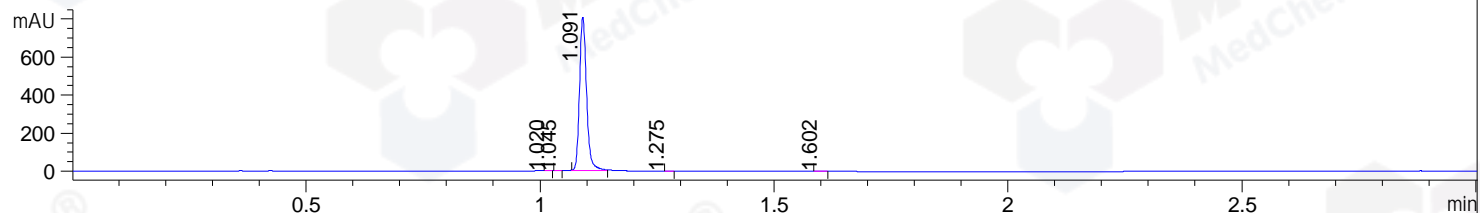

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

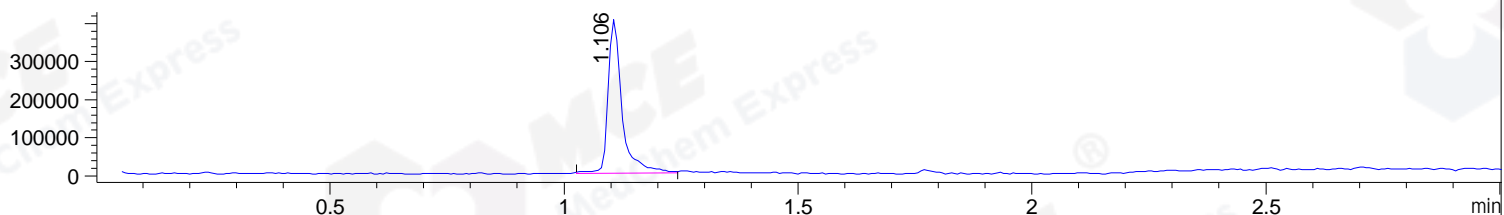

Ion 287.1, MSD1 287.1, Target Mass 286.1 +H Positive, EIC=286.8:287.8

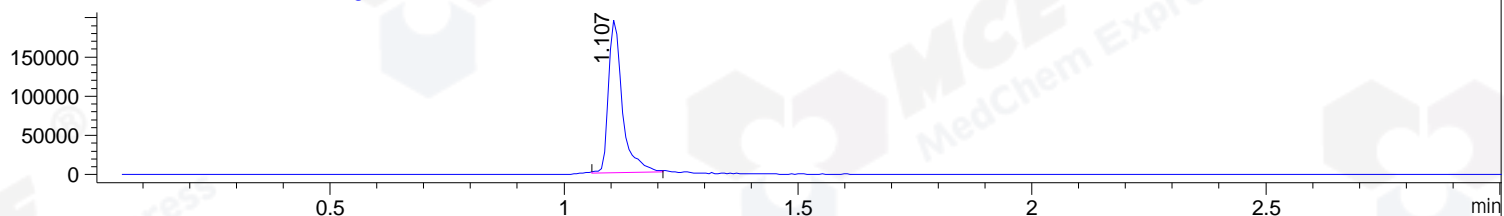

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.02	1936.08	1290.71	99.93	287
1.75	0.02	1.33	1.43	0.07	305

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.02	0.01	0.22	0.34	0.03	234
1.04	0.02	0.28	0.27	0.03	287
1.09	0.02	840.26	806.90	99.85	287
1.28	0.01	0.35	0.47	0.04	287
1.60	0.02	0.44	0.39	0.05	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.03	839908.25	403864.03	100.00	287

Ret. Time: 1.11

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

