

File ..ATA\2020\20200929\1120\BIZ2020-928-WMX11-.D Tgt Mass (CHM):

Injection Date : 29 Sep 20 3:04 pm +0800 Seq. Line : 68

Sample Name : BIZ2020-928-WMX11 Location : PL-B-05

Acq. Operator : zyj_1547 Inj : 1

Spec. Reported : MS Integration Inj Volume : 2 ul

Acq. Method : D:\Chem32\1\data\2020\20200929\1120\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200929\1120\1-POS-3MIN.M

Catalog No : HY-114855


Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)

Gradient: 5% to 95%B within 1.3 min


Flow Rate :1.8ml/min

Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

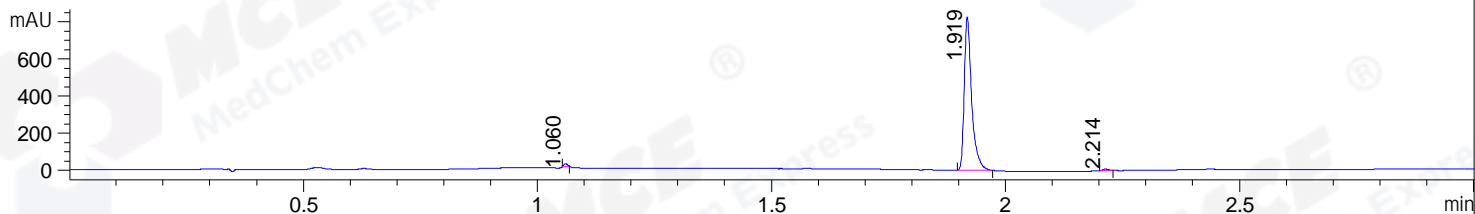


DAD1 C, Sig=254,4 Ref=off

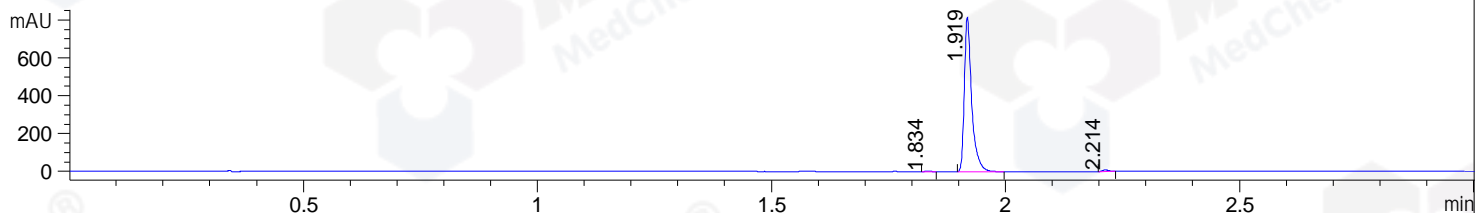

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

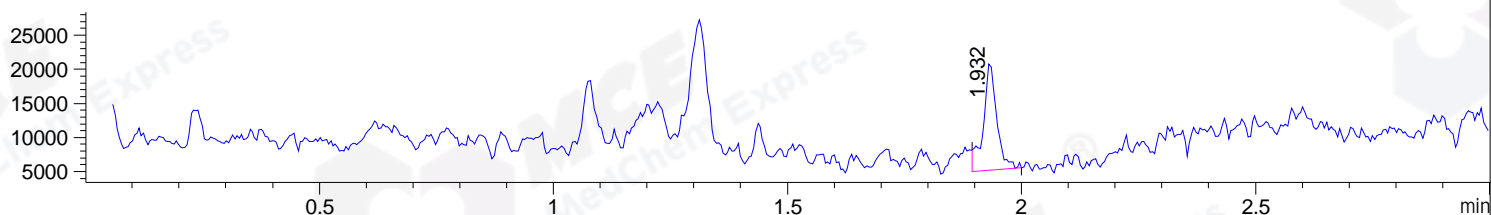

Ion 246, MSD1 246, Target Mass 245 +H Positive, EIC=245.7:246.7

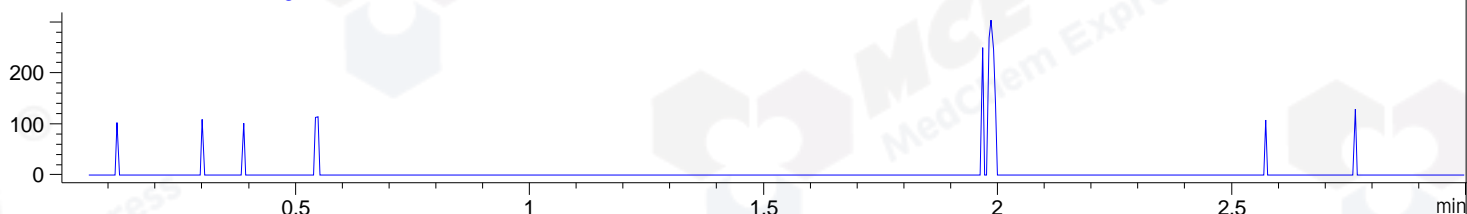

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.01	8.41	15.05	0.91	237
1.92	0.02	909.40	827.36	98.33	247
2.21	0.01	7.04	7.84	0.76	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.83	0.01	2.70	3.26	0.30	ND
1.92	0.02	894.53	816.80	98.78	247
2.21	0.02	8.36	8.21	0.92	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.93	0.03	31042.93	15797.91	100.00	247

Ret. Time: 1.93

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

