

File ..\DATA\2019\20190717\633\BIZ2019-716-WYQ8.D Tgt Mass (CHM):

Injection Date : 17 Jul 19 12:34 pm +0800 Seq. Line : 50

Sample Name : BIZ2019-716-WYQ8 Location : PI-A-08

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.4 ul

Acq. Method : D:\Chem32\1\data\2019\20190717\633\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190717\633\1-POS-3MIN.M

Catalog No : HY-120111 Batch#44165

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

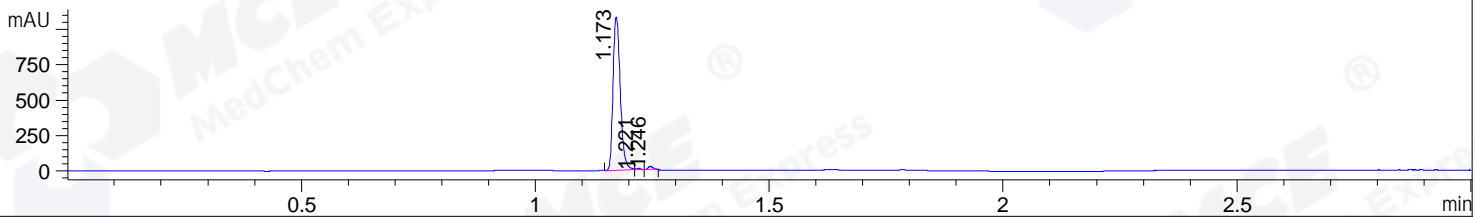


DAD1 C, Sig=254,4 Ref=off

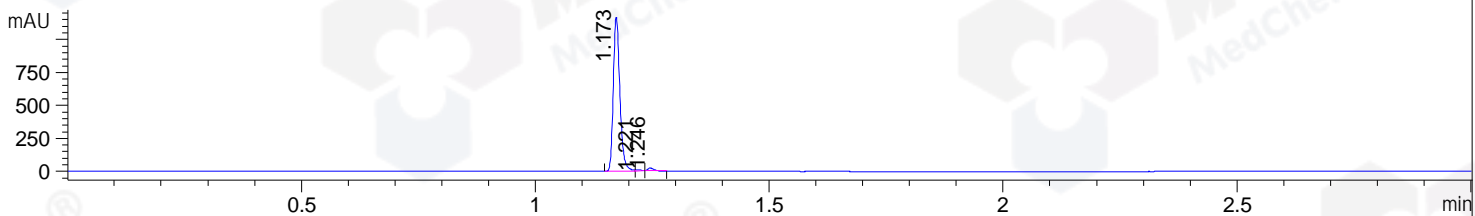

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

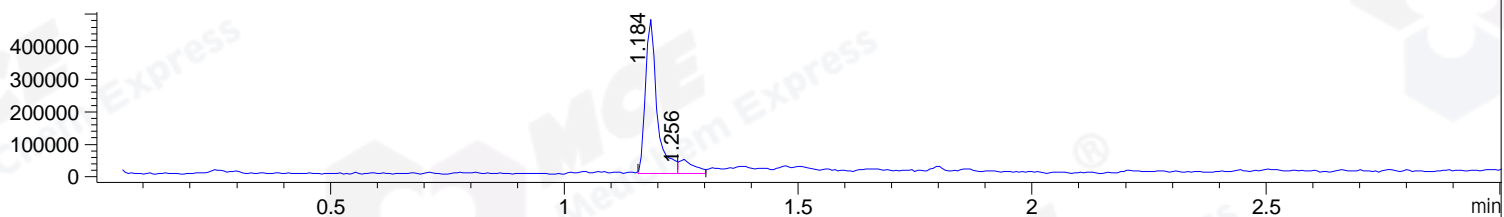

Ion 490.1, MSD1 490.1, Target Mass 489.1 +H Positive, EIC=489.8:490.8

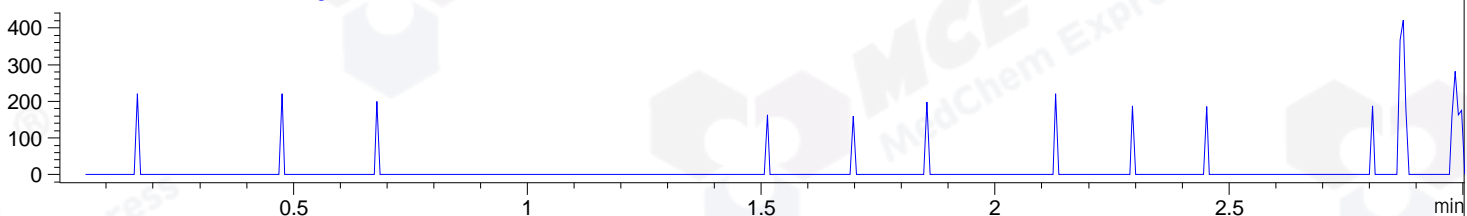

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	1160.56	1082.18	98.23	382
1.22	0.01	6.42	8.82	0.54	382
1.25	0.01	14.50	20.35	1.23	382

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	1137.17	1170.46	98.05	382
1.22	0.01	6.70	8.86	0.58	382
1.25	0.01	15.91	20.43	1.37	382

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.18	0.03	818309.06	474455.94	89.44	382
1.26	0.03	96625.67	44172.93	10.56	382

Ret. Time: 1.18

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.26

ES-API Positive

