



File ..DATA\2020\20200914\1106\CPK2020-914-05062.D Tgt Mass (CHM):
Injection Date : 14 Sep 20 8:27 pm +0800 Seq. Line : 147
Sample Name : CPK2020-914-05062 Location : P1-E-03
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200914\1106\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200914\1106\1-POS-3MIN.M
Catalog No : HY-12061
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

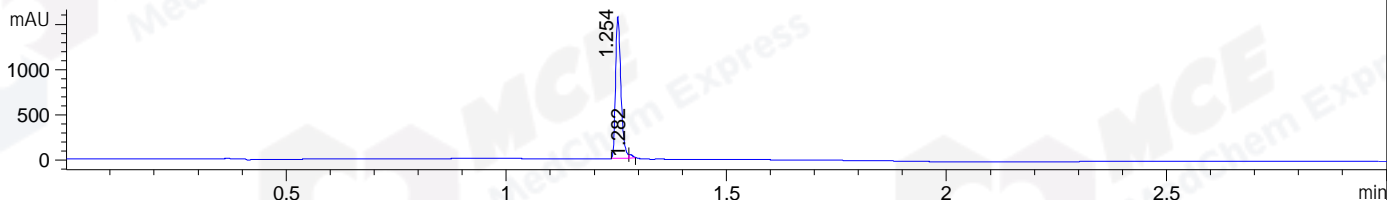


DAD1 C, Sig=254,4 Ref=off

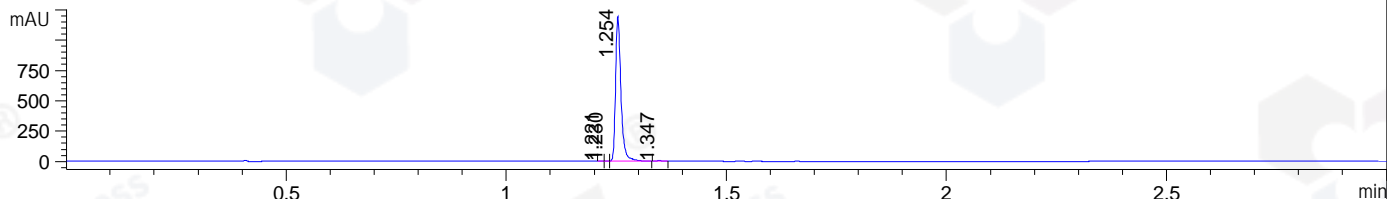

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

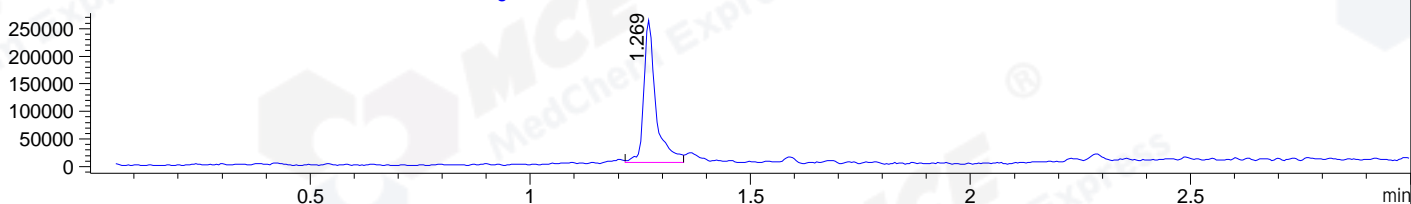

Ion 548, MSD1 548, Target Mass 547 +H Positive, EIC=547.7:548.7

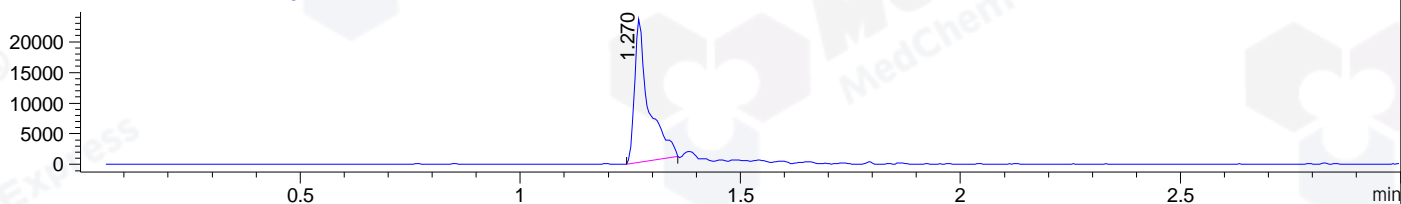

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	1324.05	1570.46	98.41	275
1.28	0.01	21.43	35.68	1.59	275

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.01	0.84	1.52	0.08	ND
1.23	0.01	1.69	2.61	0.17	635
1.25	0.01	1011.09	1195.29	99.43	275
1.35	0.01	3.25	4.09	0.32	393

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.27	0.03	494287.09	258271.00	100.00	275

Ret. Time: 1.27

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

