



File ..DATA\2020\20200814\1070\BIZ2020-812-SCH10.D Tgt Mass (CHM):  
 Injection Date : 14 Aug 20 11:15 am +0800 Seq. Line : 26  
 Sample Name : BIZ2020-812-SCH10 Location : P1-A-02  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200814\1070\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200814\1070\1-POS-3MIN.M  
 Catalog No : HY-121282A  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

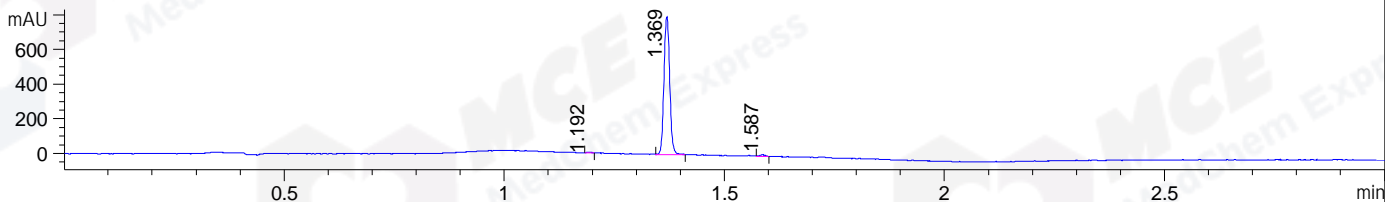


DAD1 C, Sig=254,4 Ref=off

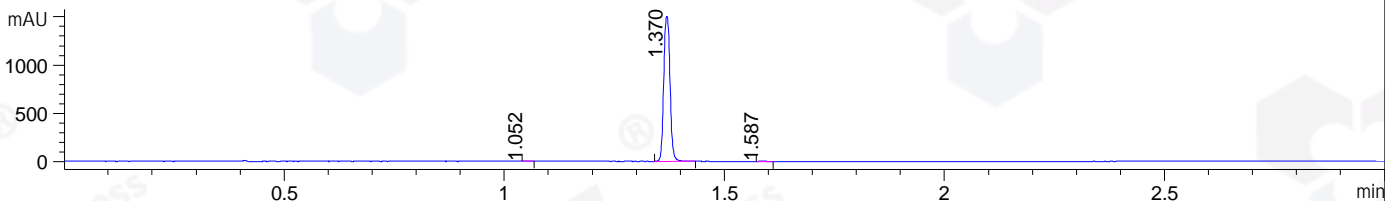

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

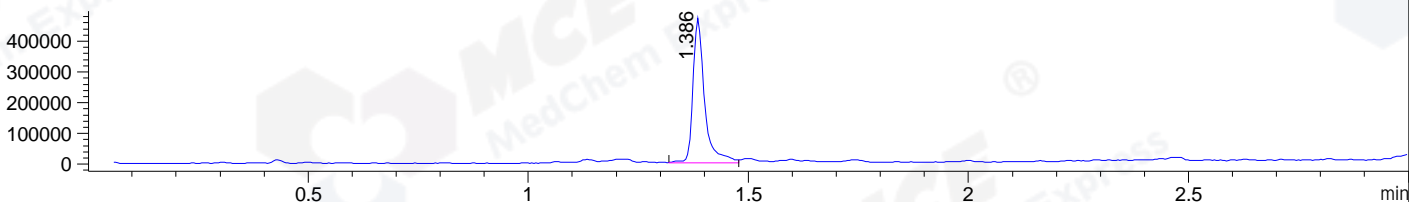

Ion 347, MSD1 347, Target Mass 346 +H Positive, EIC=346.7:347.7

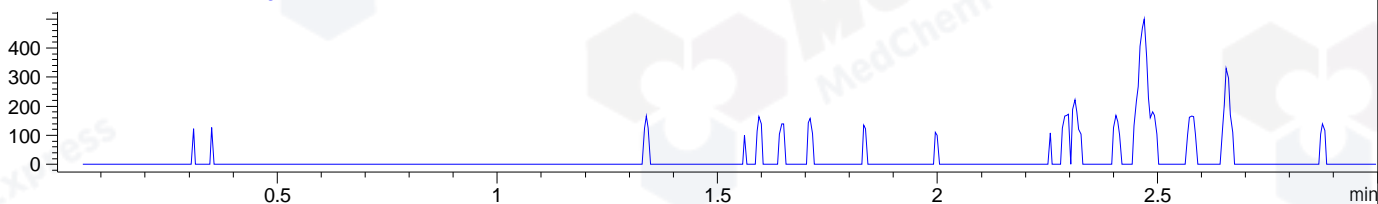

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.19	0.01	3.14	3.94	0.43	227
1.37	0.02	719.41	796.81	98.29	311
1.59	0.01	9.39	10.58	1.28	311

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.05	0.02	1.47	1.51	0.10	202
1.37	0.02	1483.60	1505.04	99.64	311
1.59	0.02	3.94	4.03	0.26	311

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.39	0.03	881165.25	471188.44	100.00	311

Ret. Time: 1.39

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

311.0 312.1 314.2