



Chromatogram and Results

Injection Details

Injection Name: CPK2020-928-04276	Run Time (min): 16.00
Vial Number: BD5	Injection Volume: 1.00
Injection Type: Unknown	Channel: UV_VIS_1
Users: ghj	Wavelength: 220
Instrument Method: 5A, 220NM	Bandwidth: 4
Processing Method: 3D Quantitative	Dilution Factor: 1.0000
Injection Date/Time: 28/Sep/2020 16:09	Sample Weight: 1
Comment: HM-073_21A-20200928 A-RP-427	

chrom://hy557/ChromeleonLocal/Instrument Data/202009/20200928.seq/459.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

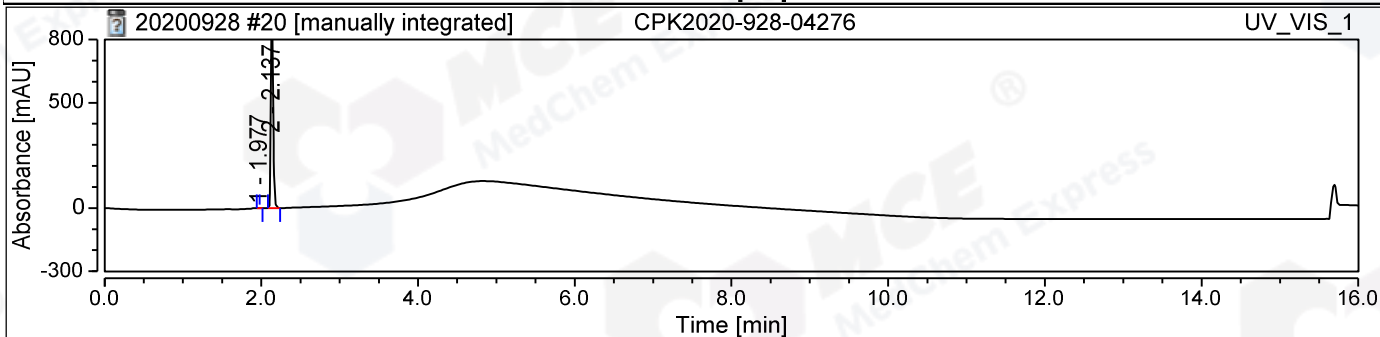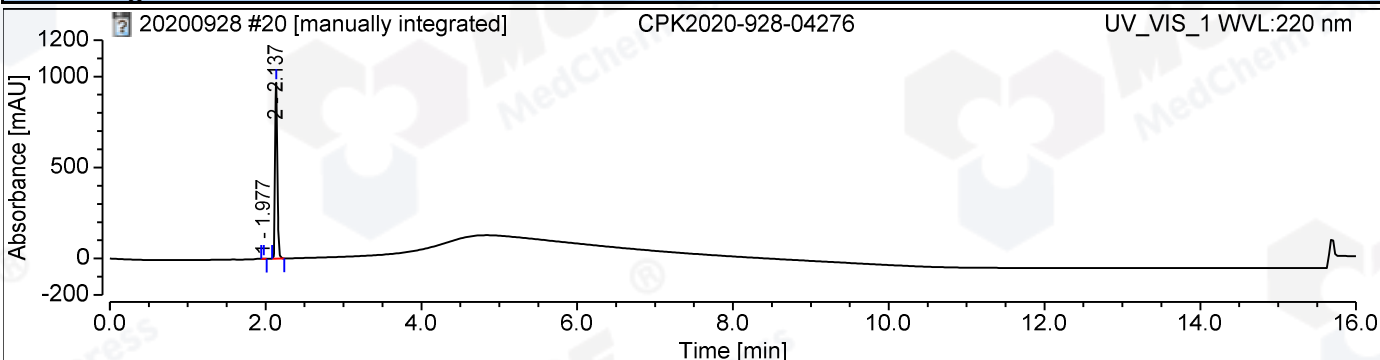

Integration Results

No.	Retention min	Area mAU*min	Height mAU	Resolution (EP)	Asymmetry (EP)	Match	Rel.Area %
1	1.98	0.007	0.186	2.72	1.04	886	0.02
2	2.14	31.698	966.563	n.a.	1.17	999	99.98
Total:			966.749	2.719	2.21	1884.73	