



File ..DATA\2020\20200708\1027\BIZ2020-707-SCH8-.D Tgt Mass (CHM):
 Injection Date : 8 Jul 20 5:08 pm +0800 Seq. Line : 83
 Sample Name : BIZ2020-707-SCH8 Location : P1-B-09
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2020\20200708\1027\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200708\1027\1-POS-3MIN.M
 Catalog No : HY-122591
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

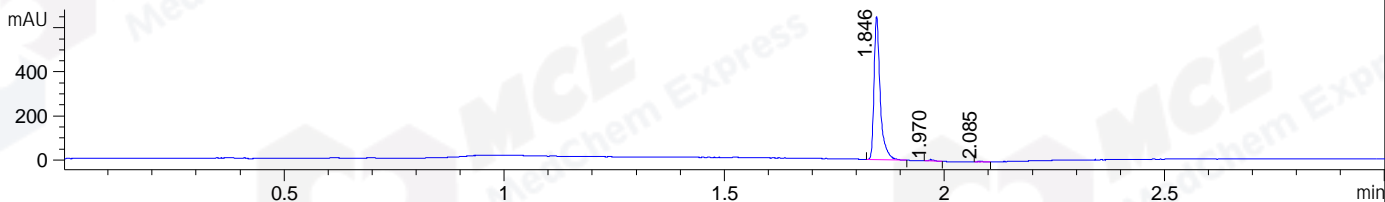


DAD1 C, Sig=254,4 Ref=off

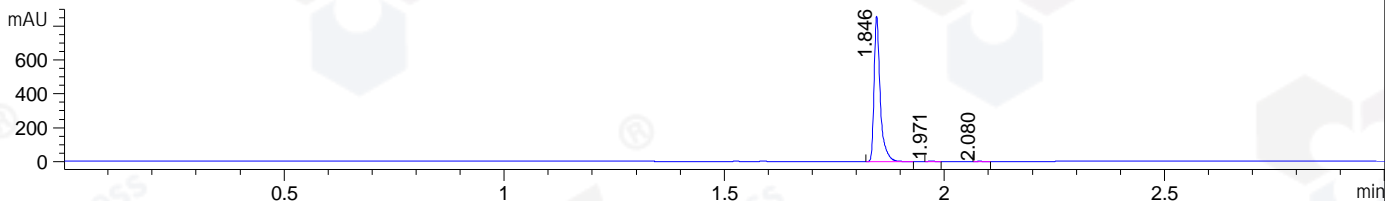

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

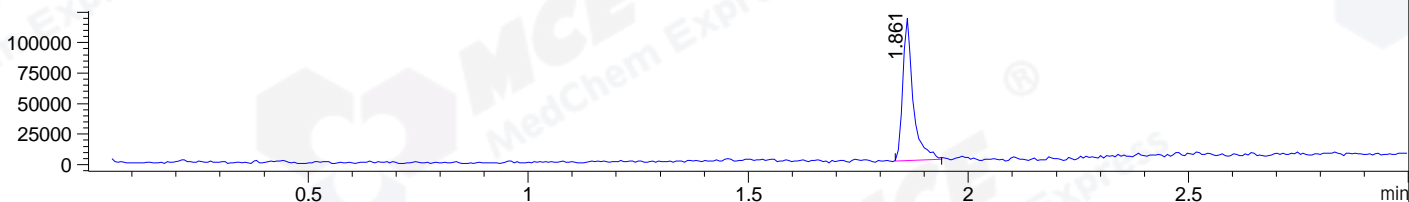

Ion 544, MSD1 544, Target Mass 543 +H Positive, EIC=543.7:544.7

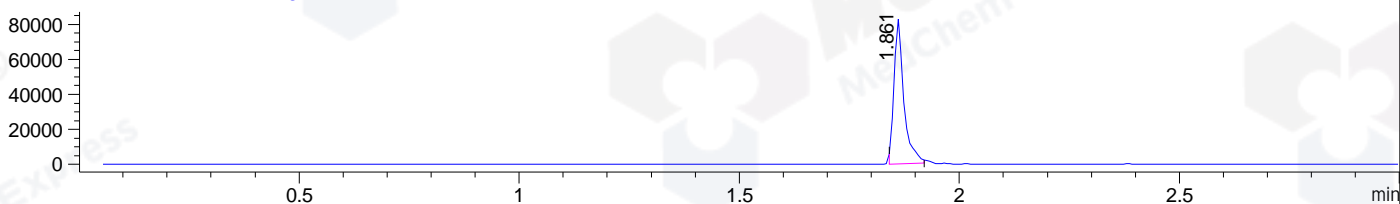

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.85	0.02	630.27	649.66	98.82	544
1.97	0.01	5.23	5.98	0.82	ND
2.08	0.02	2.26	2.06	0.36	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.85	0.02	838.85	862.48	98.98	544
1.97	0.01	4.91	5.46	0.58	ND
2.08	0.02	3.76	3.63	0.44	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.86	0.03	192365.77	116558.94	100.00	544

Ret. Time: 1.86

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



544.2

545.1

546.0