


=====  
Acq. Operator : Li Shan(LCMS-02) Seq. Line : 24  
Acq. Instrument : HY-LCMS-02 Location : P1-C-06  
Injection Date : 4/13/2015 11:08:45 AM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20150413\20150413 2015-04-13 09-29-04\100-1000MS+3MIN-1.5\_(0.02%FA).M  
Last changed : 4/13/2015 9:29:04 AM by Li Shan(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20150202\20150202 2015-02-02 09-14-27\100-1000MS+3MIN(0.02%FA).M (Sequence Method)  
Last changed : 4/13/2015 12:57:46 PM by Li Shan(LCMS-02)  
(modified after loading)  
Method Info : Postive,MS:100-1000,Column ID:A-RP-102,40°C  
Catalog No : HY-12289 Batch#15678  
A-RP-132

Additional Info : Peak(s) manually integrated

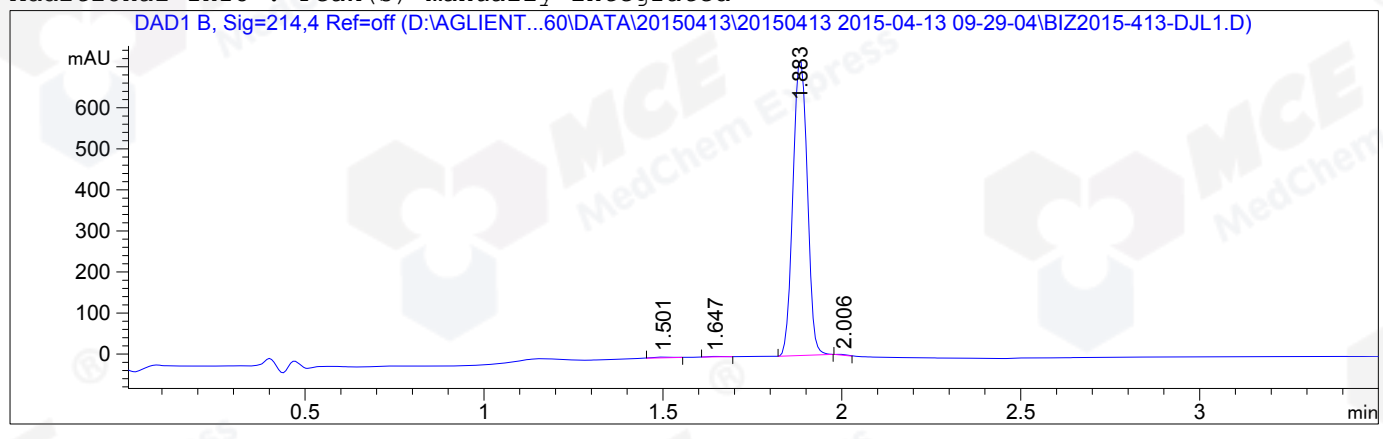

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=214,4 Ref=off


Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.501	MM	0.0616	7.30582	1.97584	0.3616
2	1.647	MM	0.0432	2.72954	1.05217	0.1351
3	1.883	MM	0.0461	2006.90625	725.92889	99.3185
4	2.006	MM	0.0325	3.73580	1.91378	0.1849

Totals : 2020.67741 730.87068

=====  
\*\*\* End of Report \*\*\*


=====  
Acq. Operator : Li Shan(LCMS-02) Seq. Line : 24  
Acq. Instrument : HY-LCMS-02 Location : P1-C-06  
Injection Date : 4/13/2015 11:08:45 AM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20150413\20150413 2015-04-13 09-29-04\100-1000MS+3MIN-  
1.5\_(0.02%FA).M  
Last changed : 4/13/2015 9:29:04 AM by Li Shan(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20150202\20150202 2015-02-02 09-14-27\100-1000MS+3MIN(  
0.02%FA).M (Sequence Method)  
Last changed : 4/13/2015 12:59:24 PM by Li Shan(LCMS-02)  
(modified after loading)  
Method Info : Postive,MS:100-1000,Column ID:A-RP-102,40°C  
Catalog No : HY-12289 Batch#15678  
A-RP-132

Additional Info : Peak(s) manually integrated

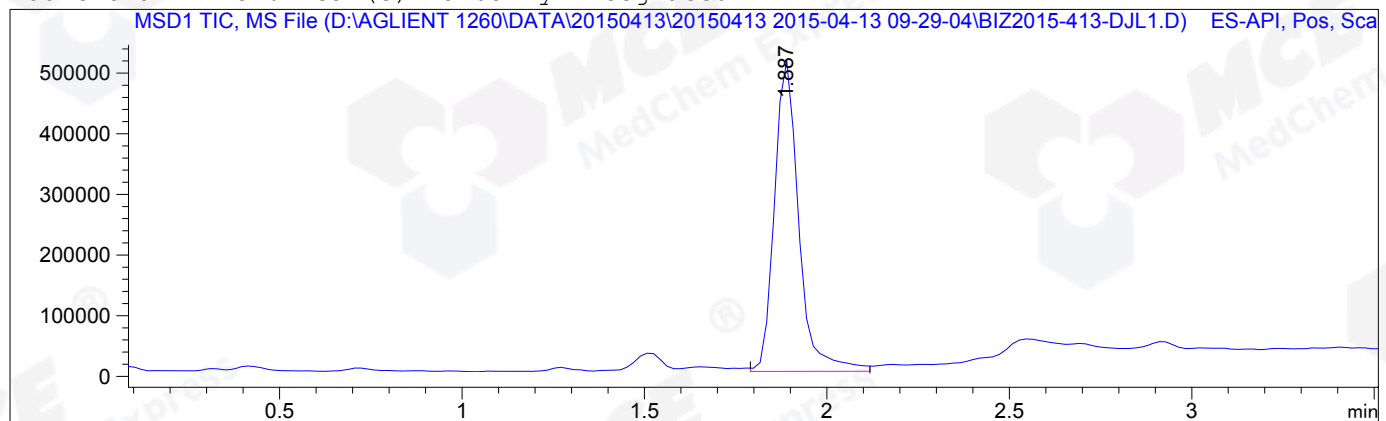

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50  
Spectra averaged over upper half of peaks.  
Noise Cutoff: 1000 counts.  
Reportable Ion Abundance: > 10%.

Retention Time (MS)	MS Area	Mol. Weight or Ion
1.887	2374080	511.80 I
		510.80 I

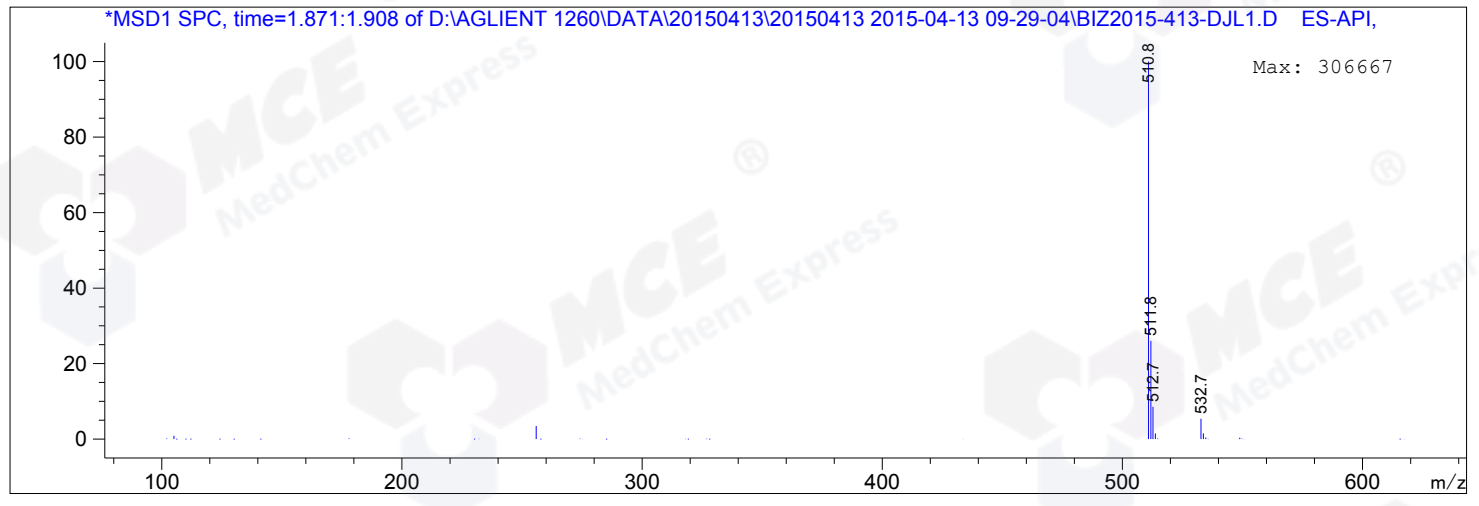

\*\*\* End of Report \*\*\*