

File ..1\DATA\2020\20200416\927\BIZ2020-415-SCH7.D Tgt Mass (CHM):

Injection Date : 16 Apr 20 4:27 pm +0800 Seq. Line : 96

Sample Name : BIZ2020-415-SCH7 Location : PL-C-09

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200416\927\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200416\927\1-POS-3MIN.M

Catalog No : HY-123054

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

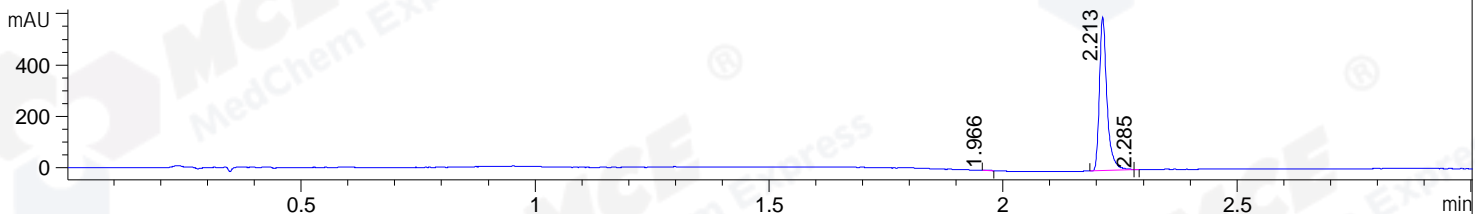


DAD1 C, Sig=254,4 Ref=off

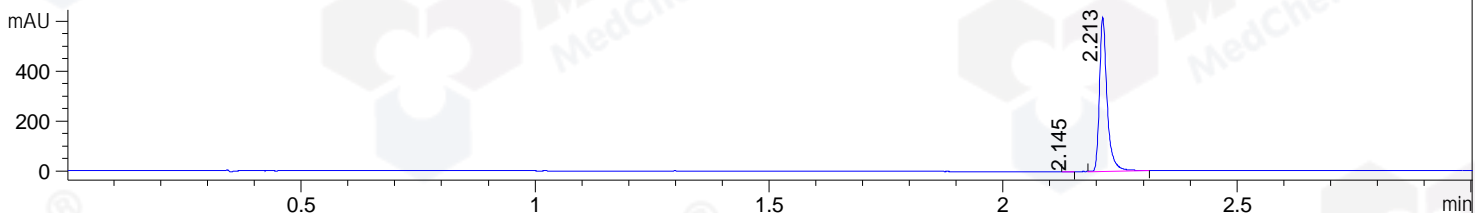

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

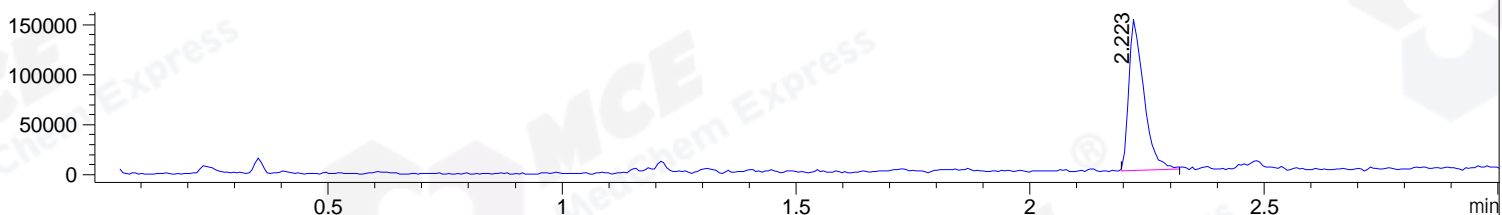

Ion 431, MSD1 431, Target Mass 430 +H Positive, EIC=430.7:431.7

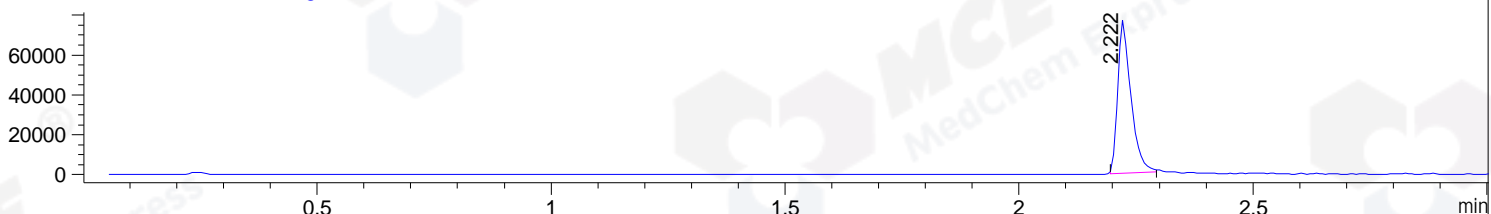

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.97	0.01	1.22	1.60	0.18	ND
2.21	0.02	673.11	598.78	99.74	431
2.29	0.01	0.54	1.13	0.08	431

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.15	0.01	0.41	0.52	0.06	ND
2.21	0.02	702.48	618.25	99.94	431

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.22	0.04	337665.72	150917.42	100.00	431

Ret. Time: 2.22

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

