

File ..ATA\2020\20200711\1034\CPK2020-710-14938-.D Tgt Mass (CHM):

Injection Date : 11 Jul 20 2:24 pm +0800 Seq. Line : 16

Sample Name : CPK2020-710-14938 Location : P1-D-02

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.5 ul

Acq. Method : D:\Chem32\1\data\2020\20200711\1034\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200711\1034\1-POS-3MIN.M

Catalog No : HY-12335

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

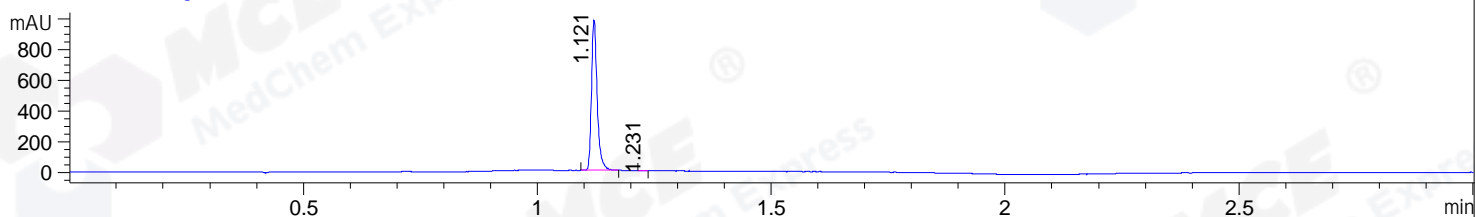


DAD1 C, Sig=254,4 Ref=off

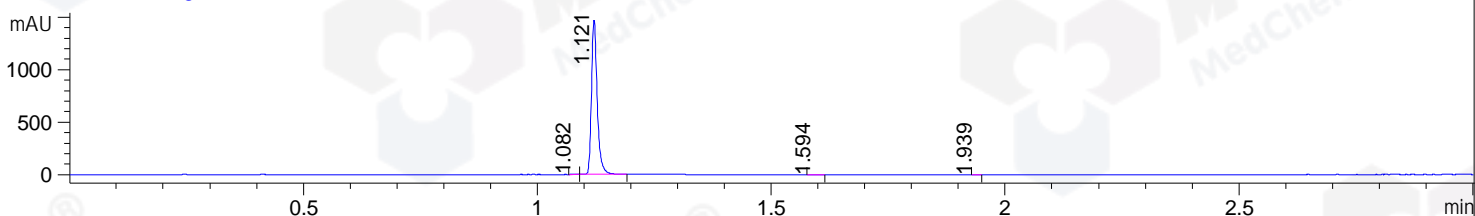

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

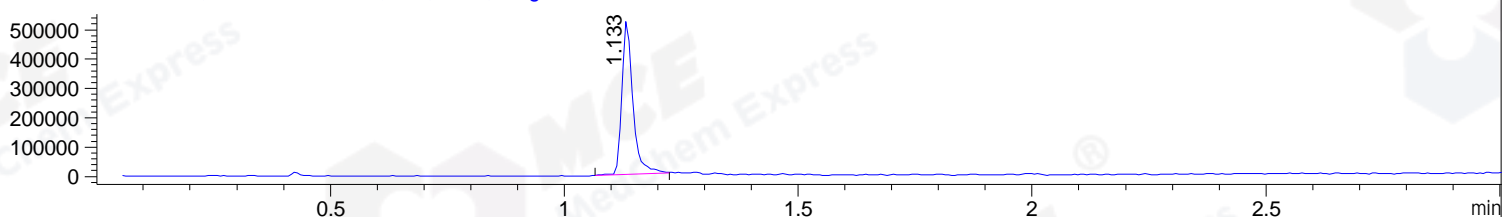

Ion 414, MSD1 414, Target Mass 413 +H Positive, EIC=413.7:414.7

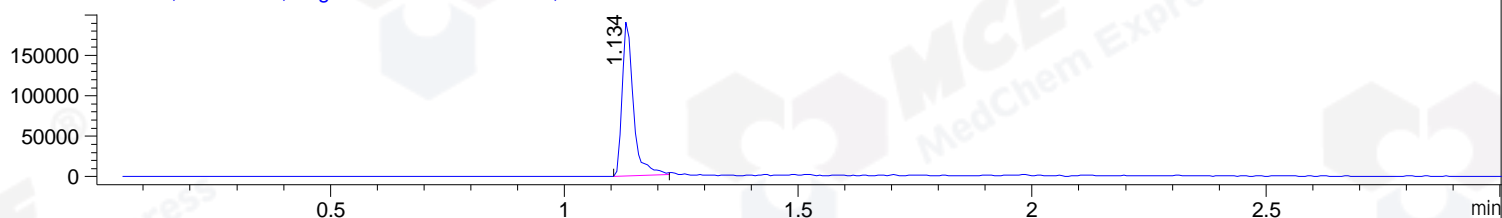

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.01	821.99	979.70	99.83	208
1.23	0.01	1.42	1.86	0.17	414

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.01	1.60	1.89	0.13	ND
1.12	0.01	1249.62	1473.25	99.75	208
1.59	0.02	1.18	1.13	0.09	414
1.94	0.01	0.35	0.72	0.03	414

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.03	866469.38	524555.38	100.00	208

Ret. Time: 1.13

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

