



File ..DATA\2020\20200919\1111\CPK2020-915-13603.D Tgt Mass (CHM):
Injection Date : 19 Sep 20 5:26 pm +0800 Seq. Line : 85
Sample Name : CPK2020-915-13603 Location : P1-B-01
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200919\1111\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200919\1111\1-POS-3MIN.M
Ecvcnqi"Pq""<"J[/34586C
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

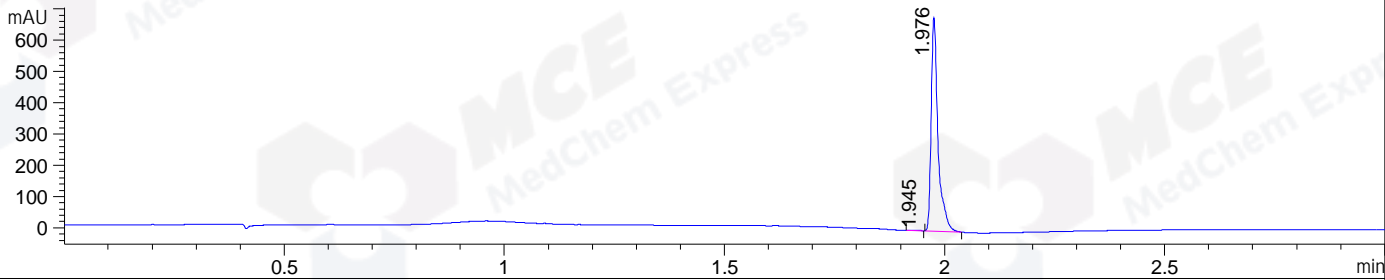

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

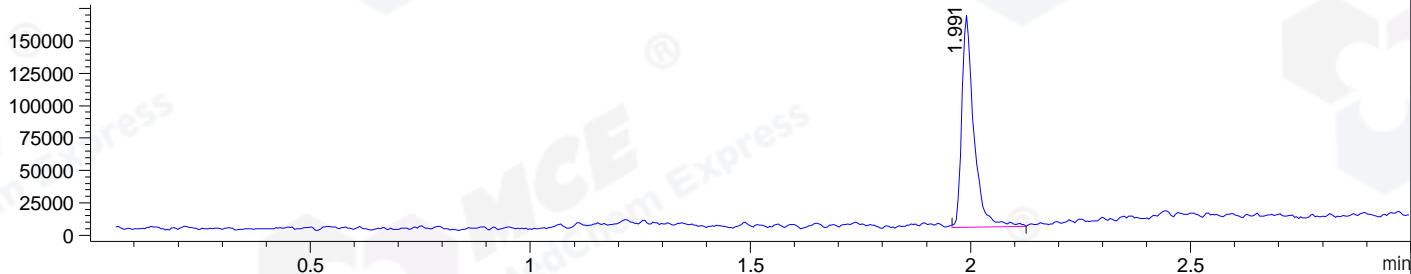

Ion 255, MSD1 255, Target Mass 254 +H Positive, EIC=254.7:255.7

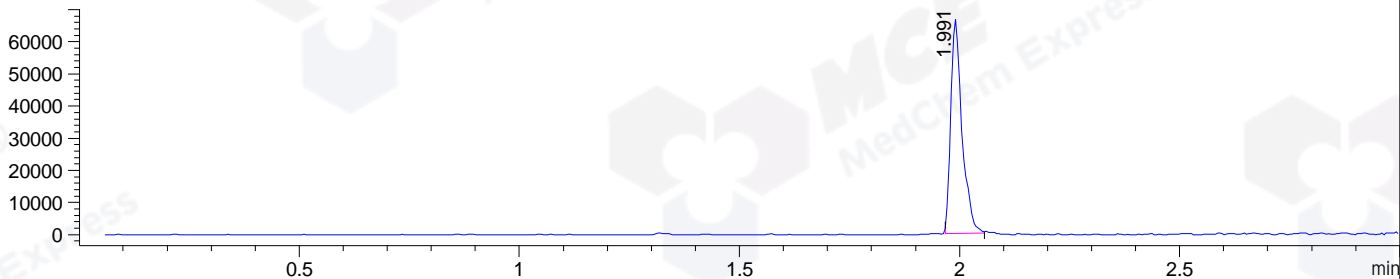

Integration Results for DAD1 B, Sig=214,4 Ref=off

| RetTim | Width | Area | Height | Area% | MS(+) |
|--------|-------|--------|--------|-------|-------|
| 1.95 | 0.03 | 0.64 | 0.41 | 0.09 | 137 |
| 1.98 | 0.02 | 735.87 | 681.75 | 99.91 | 255 |

Integration Results for MSD1 TIC, MS File

| RetTim | Width | Area | Height | Area% | MS(+) |
|--------|-------|-----------|-----------|--------|-------|
| 1.99 | 0.03 | 313555.78 | 163774.70 | 100.00 | 255 |

Ret. Time: 1.99

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

