



File ..DATA\2020\20200724\1052\BIZ2020-723-SCH8-.D Tgt Mass (CHM):  
Injection Date : 24 Jul 20 12:46 pm +0800 Seq. Line : 51  
Sample Name : BIZ2020-723-SCH8 Location : P1-B-05  
Acq. Operator : ZJ\_1432 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 0.5 ul  
Acq. Method : D:\Chem32\1\data\2020\20200724\1052\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200724\1052\1-POS-3MIN.M  
Catalog No : HY-123673  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

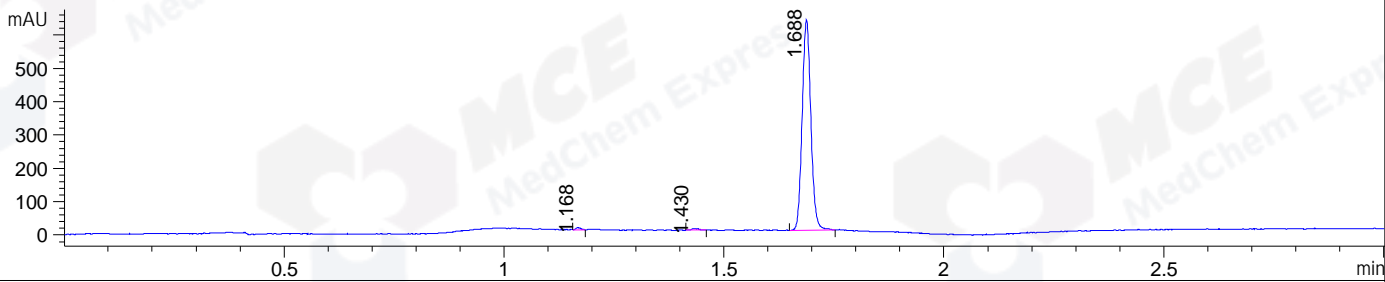

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

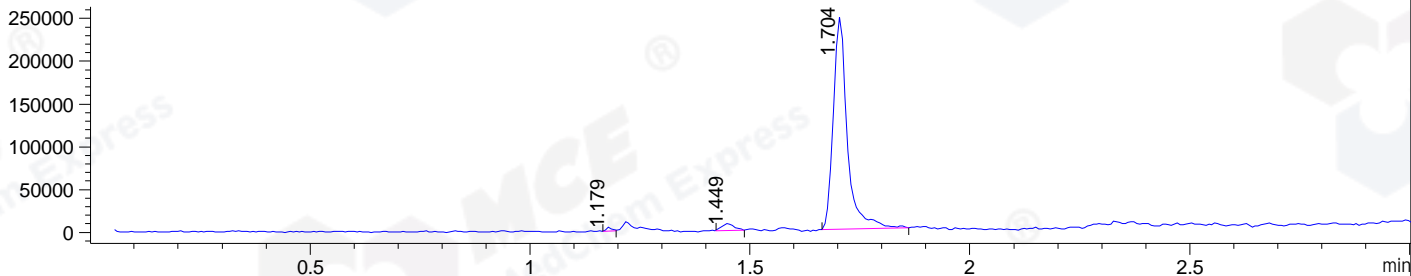

Ion 509, MSD1 509, Target Mass 508 +H Positive, EIC=508.7:509.7

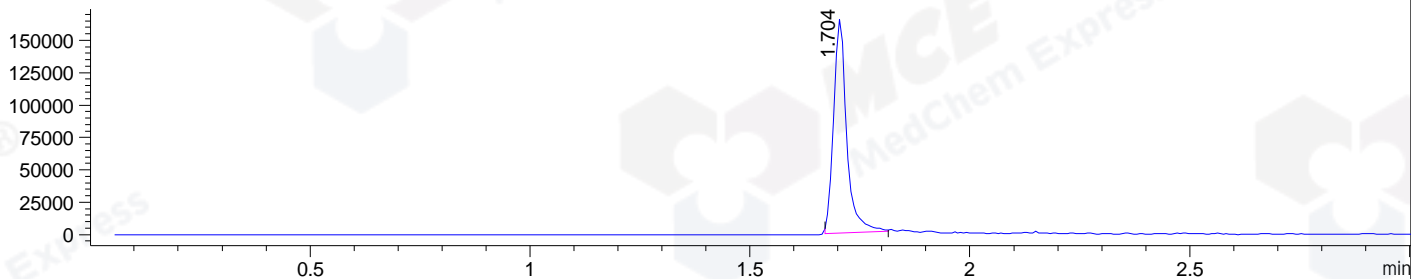

Integration Results for DAD1 B, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.01	4.96	6.23	0.56	ND
1.43	0.02	4.61	3.81	0.52	247
1.69	0.02	869.62	631.32	98.91	509

Integration Results for MSD1 TIC, MS File


RetTim	Width	Area	Height	Area%	MS (+)
1.18	0.01	3901.95	4653.79	0.69	136
1.45	0.03	16724.51	8704.18	2.95	247
1.70	0.03	546016.63	247625.73	96.36	509

Ret. Time: 1.18

<<<< POSITIVE SPECTRA >>>>

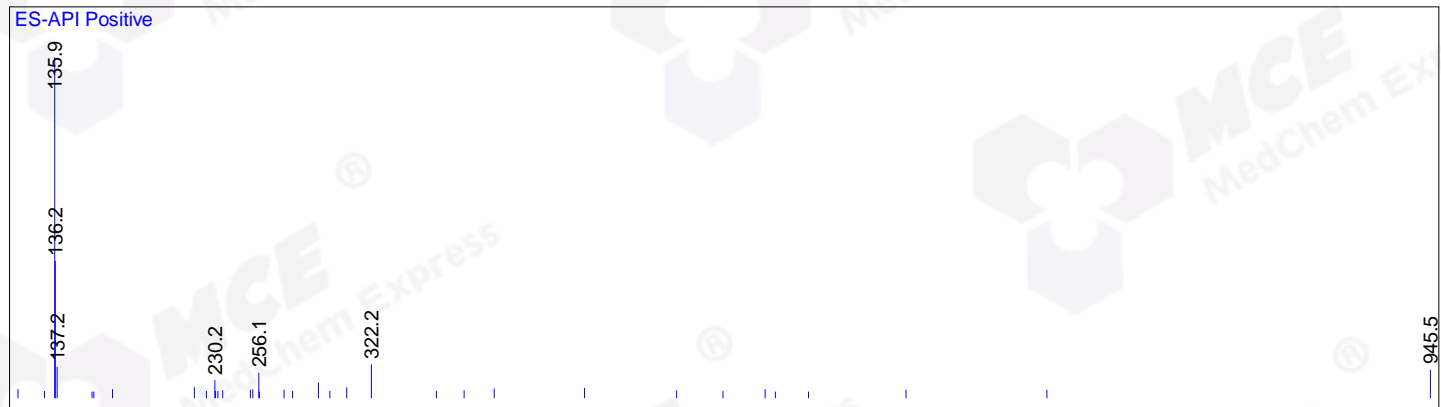

Ret. Time: 1.45

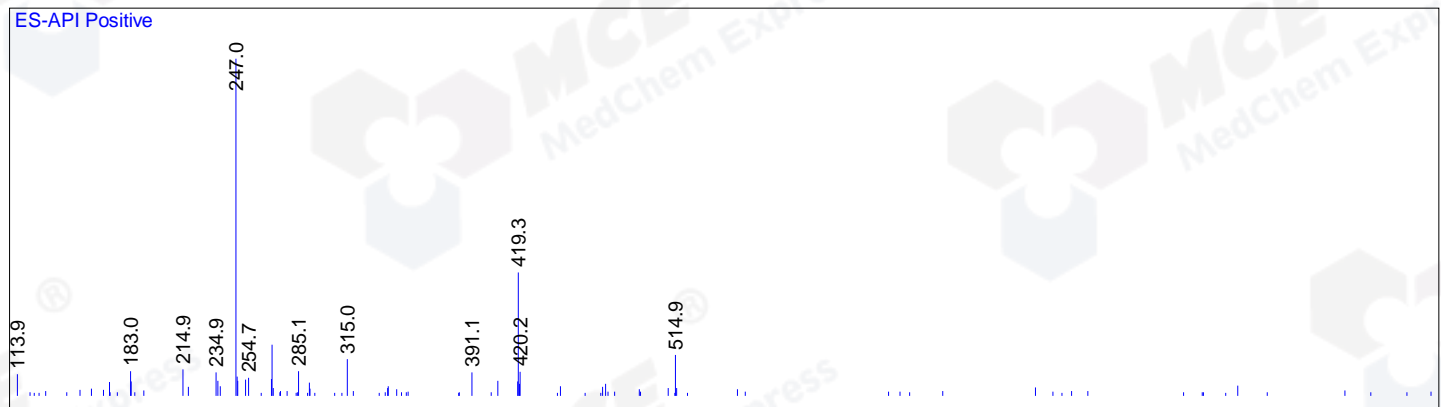

Ret. Time: 1.70

