
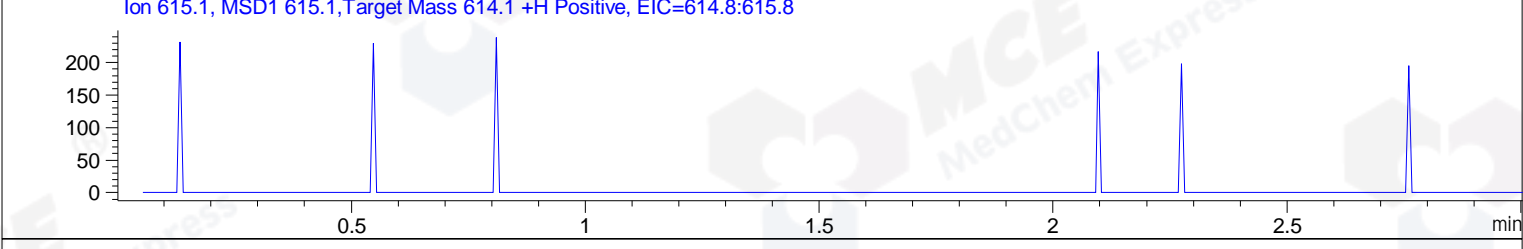
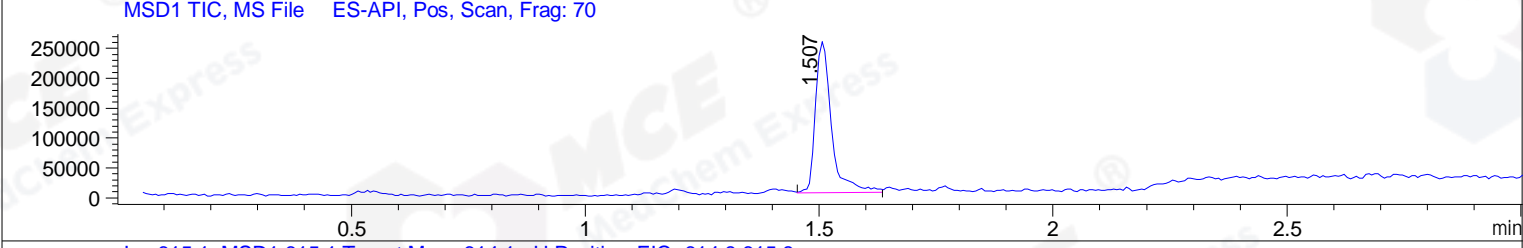
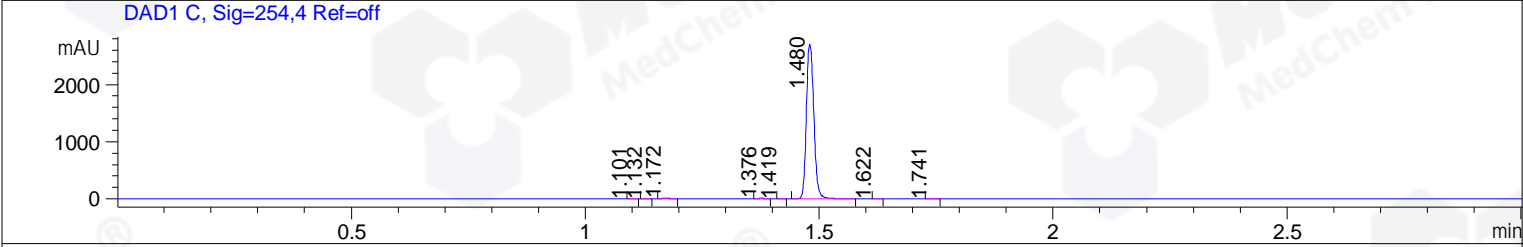


File ..1\DATA\2018\20181226\551\BIZ2018-D26-CXL1.D Tgt Mass (CHM):
 Injection Date : 26 Dec 18 5:21 pm +0800 Seq. Line : 30
 Sample Name : BIZ2018-D26-CXL1 Location : P1-B-02
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2018\20181226\551\1-POS-3MIN-1.M
 Analysis Method : D:\CHEM32\1\DATA\2018\20181226\551\1-POS-3MIN-1.M
 Catalog No : HY-12423A Batch#36116
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45

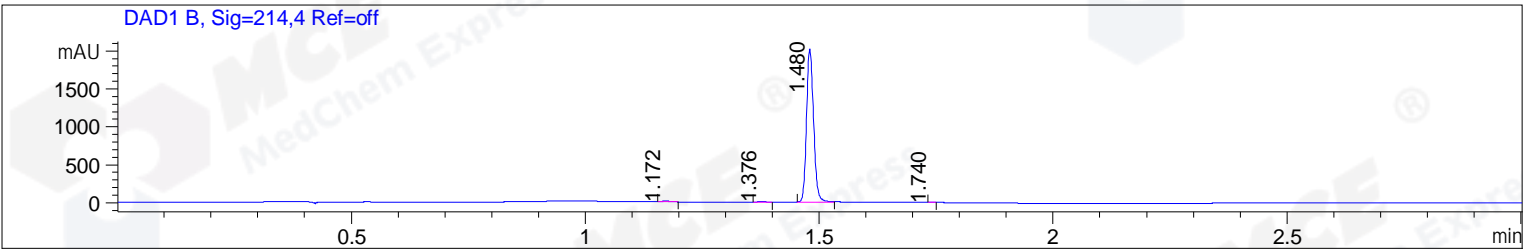

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	12.58	13.31	0.59	401
1.38	0.02	4.59	4.47	0.22	ND
1.48	0.02	2111.85	2017.86	99.15	519
1.74	0.01	0.93	1.21	0.04	519

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.01	0.78	0.93	0.03	ND
1.13	0.01	0.83	1.07	0.03	ND
1.17	0.01	16.66	18.27	0.55	401
1.38	0.02	8.14	8.48	0.27	ND
1.42	0.01	0.31	0.46	0.01	482
1.48	0.02	3013.01	2708.50	99.06	519
1.62	0.01	0.66	0.88	0.02	519
1.74	0.02	1.23	1.11	0.04	519

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.04	607880.31	253032.48	100.00	519

Ret. Time: 1.51

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

