



File ..\DATA\2020\20200813\1068\BIZ2020-811-WMX4.D Tgt Mass (CHM):
 Injection Date : 13 Aug 20 11:30 am +0800 Seq. Line : 32
 Sample Name : BIZ2020-811-WMX4 Location : P1-A-08
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200813\1068\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200813\1068\1-POS-3MIN.M
 Catalog No : HY-12469
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

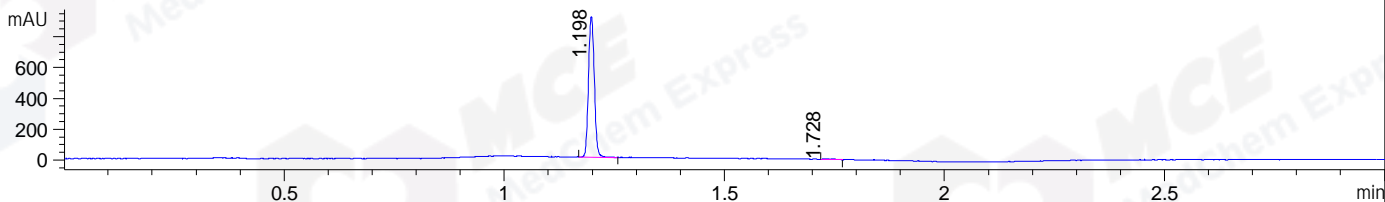


DAD1 C, Sig=254,4 Ref=off

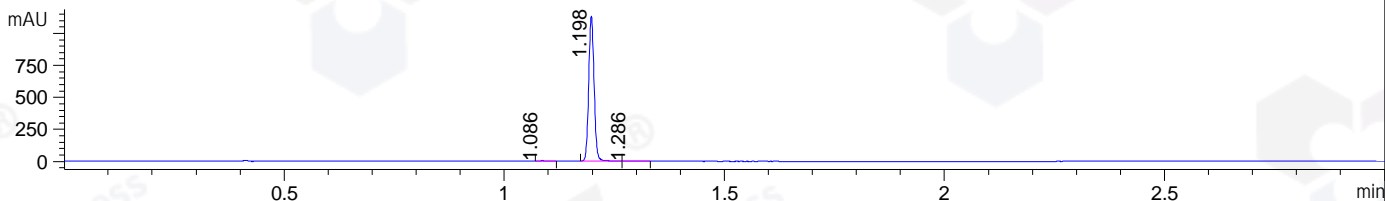

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

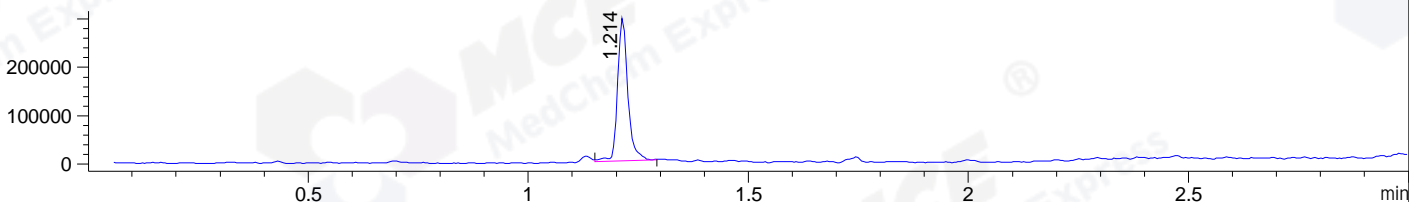

Ion 393, MSD1 393, Target Mass 392 +H Positive, EIC=392.7:393.7

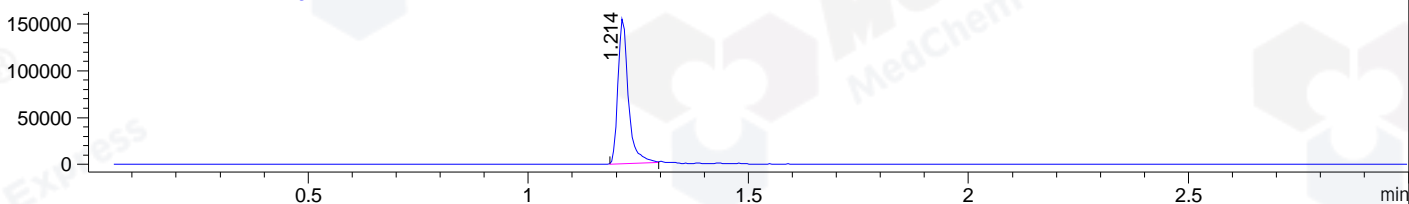

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.02	841.54	912.12	99.45	393
1.73	0.03	4.66	2.72	0.55	279

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.02	3.02	2.24	0.31	ND
1.20	0.01	959.74	1132.02	99.29	393
1.29	0.03	3.89	1.95	0.40	393

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.03	476888.03	295087.75	100.00	393

Ret. Time: 1.21

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

