



File ..1\DATA\2020\20200422\935\BIZ2020-421-CXL2.D Tgt Mass (CHM):
 Injection Date : 22 Apr 20 11:25 am +0800 Seq. Line : 32
 Sample Name : BIZ2020-421-CXL2 Location : P1-A-06
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200422\935\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200422\935\1-POS-3MIN.M
 Catalog No : HY-124745
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

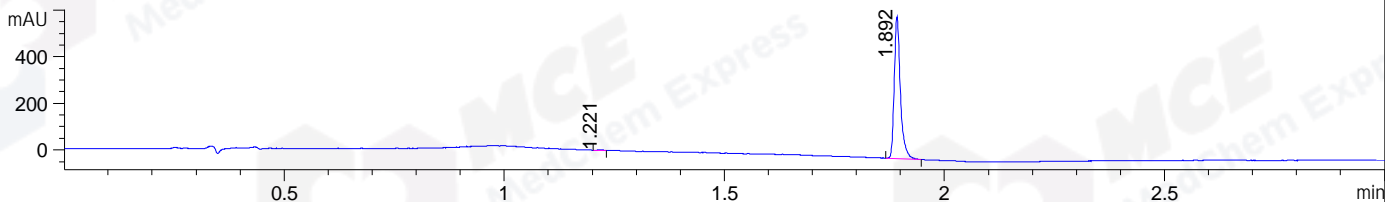


DAD1 C, Sig=254,4 Ref=off

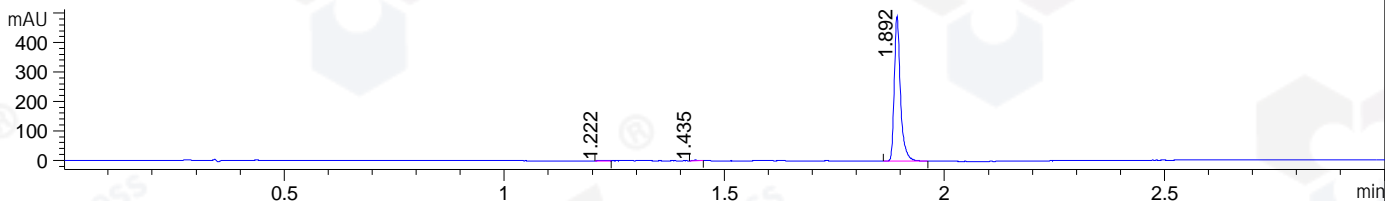

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

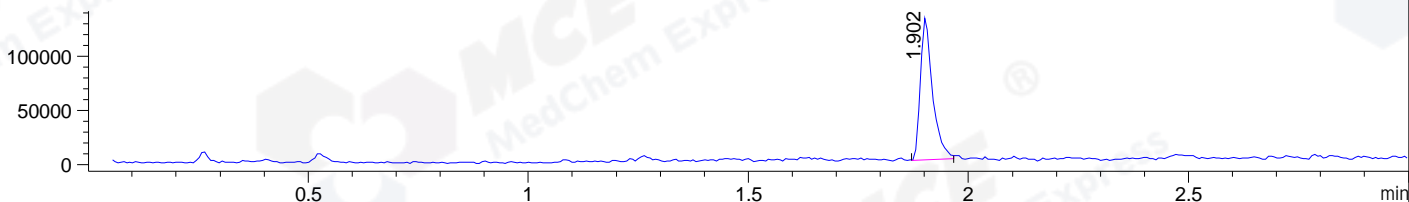

Ion 353, MSD1 353, Target Mass 352 +H Positive, EIC=352.7:353.7

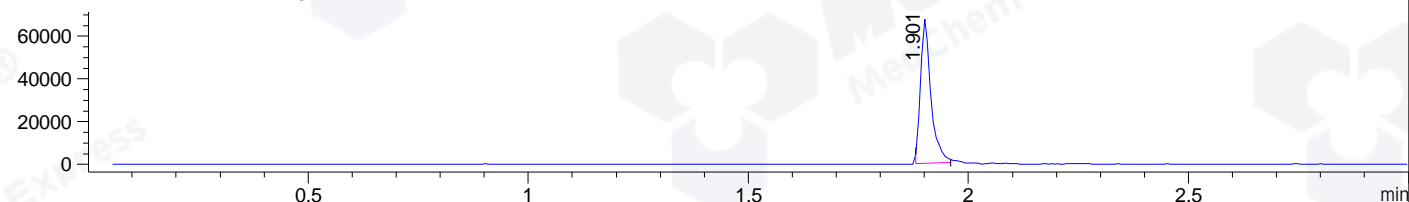

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.01	1.19	1.55	0.20	ND
1.89	0.02	593.38	610.30	99.80	353

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.02	0.97	1.01	0.20	ND
1.43	0.01	1.49	2.11	0.31	ND
1.89	0.02	480.58	492.30	99.49	353

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.90	0.03	253396.63	132448.44	100.00	353

Ret. Time: 1.90

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

