


### Chromatogram and Results

#### Injection Details

Injection Name:	ZFX5535-030-1	Injection Volume:	5.00
Vial Number:	GA5	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	254
Calibration Level:		Users:	ZLL
Instrument Method:	HM-465C_8-H01P01(RP-HPLC)	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	03/Jul/18 21:41		
Catalog No:	HY-12512 Batch#31348 A-RP-194		

chrom://hy261/ChromeleonLocal/Chemistry Analy/20180701/20180703-1.seq/703.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

#### Chromatogram

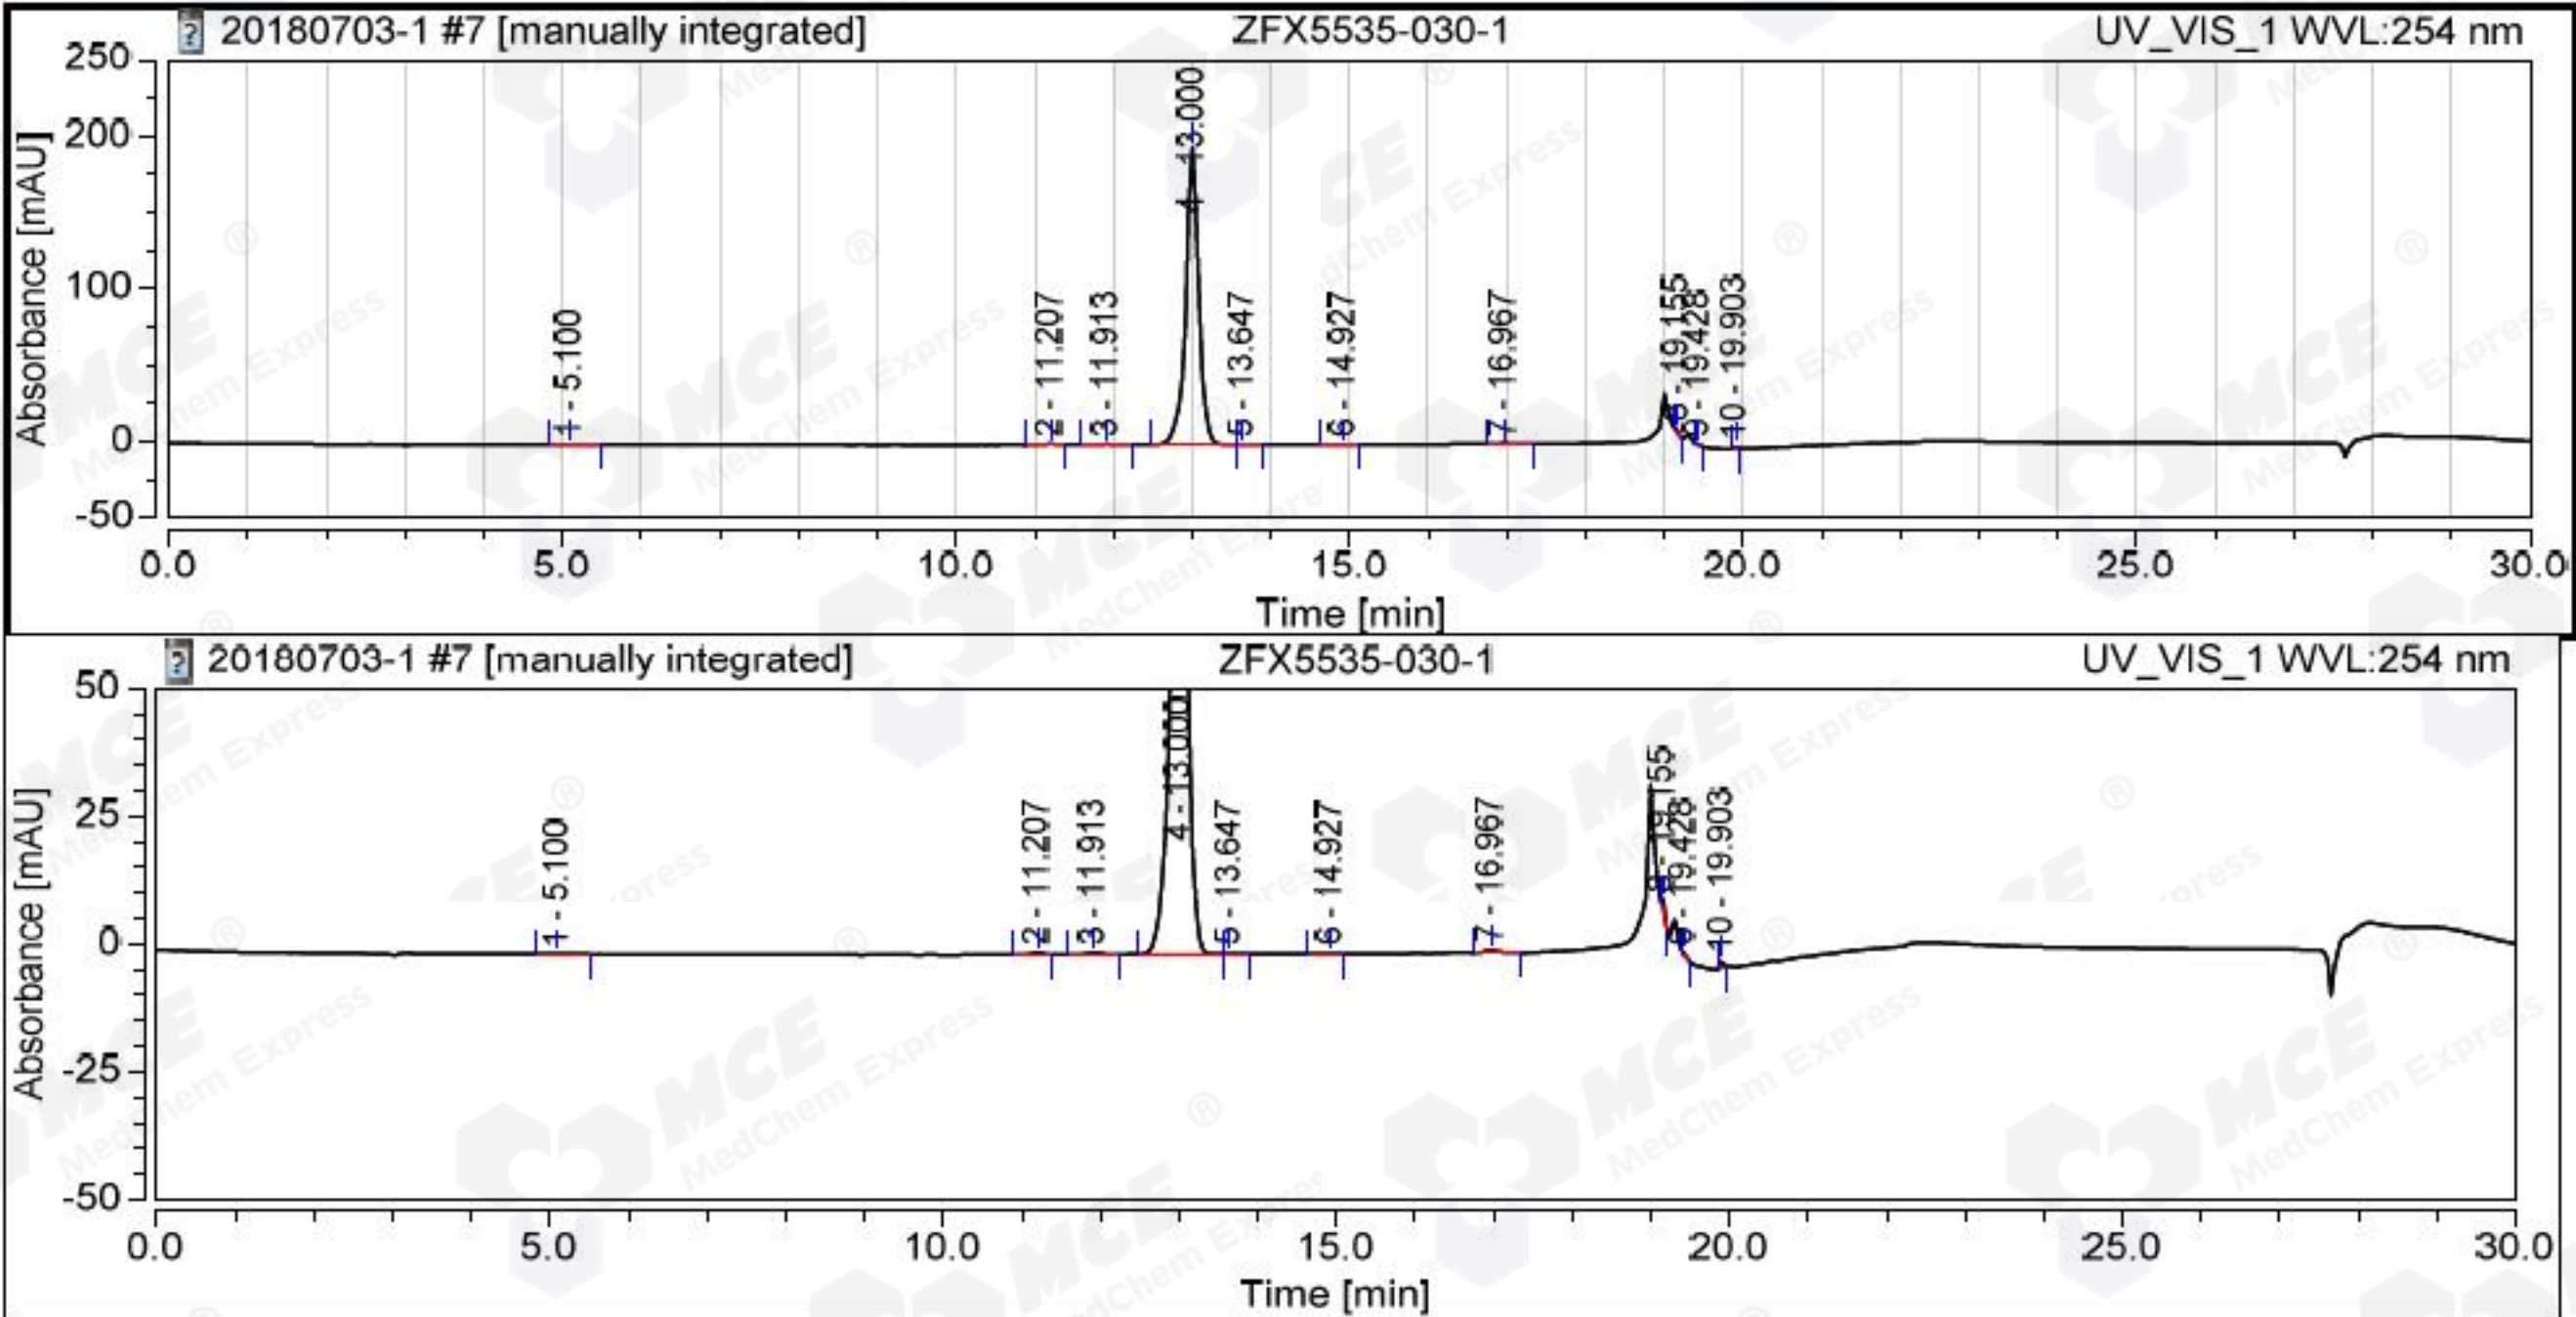

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		5.100	0.026	0.125	1.34	21.93	0.07
2		11.207	0.070	0.471	0.92	2.69	0.19
3		11.913	0.074	0.386	0.97	3.88	0.20
4		13.000	36.886	194.770	0.95	2.32	98.56
5		13.647	0.018	0.121	n.a.	4.22	0.05
6		14.927	0.026	0.140	0.89	7.16	0.07
7		16.967	0.100	0.524	1.40	13.53	0.27
8		19.155	0.113	2.551	1.57	3.88	0.30
9		19.428	0.041	0.974	1.33	6.63	0.11
10		19.903	0.073	1.644	1.12	n.a.	0.19
Total:			37.425	201.707	10.50	66.22	