

File ..\DATA\2019\20190311\553\BIZ2019-308-WYQ18.D Tgt Mass (CHM):

Injection Date : 11 Mar 19 11:44 am +0800 Seq. Line : 26

Sample Name : BIZ2019-308-WYQ18 Location : P2-E-06

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190311\553\1-POS-3MIN-1(110-1500).M

Analysis Method : D:\CHEM32\1\DATA\2019\20190311\553\1-POS-3MIN-1(110-1500).M

Catalog No : HY-12551A Batch# 38795-20190308

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

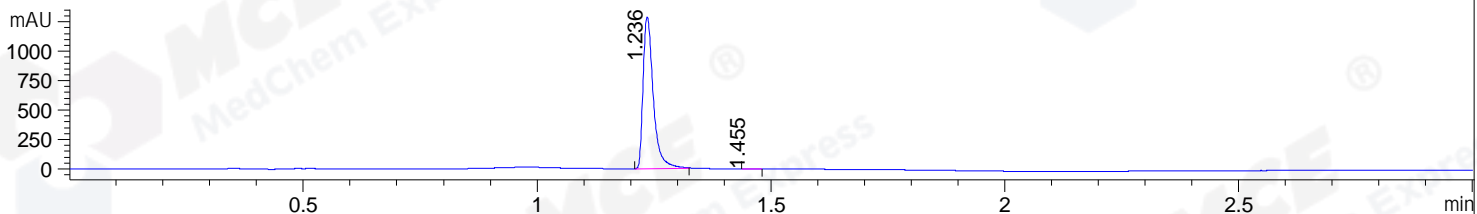


DAD1 C, Sig=254,4 Ref=off

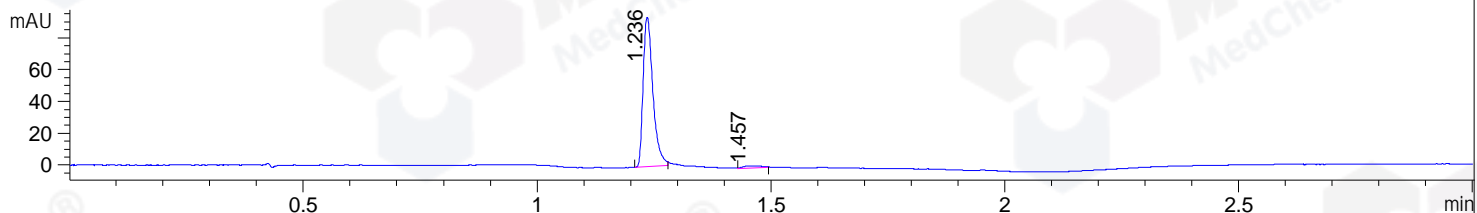

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

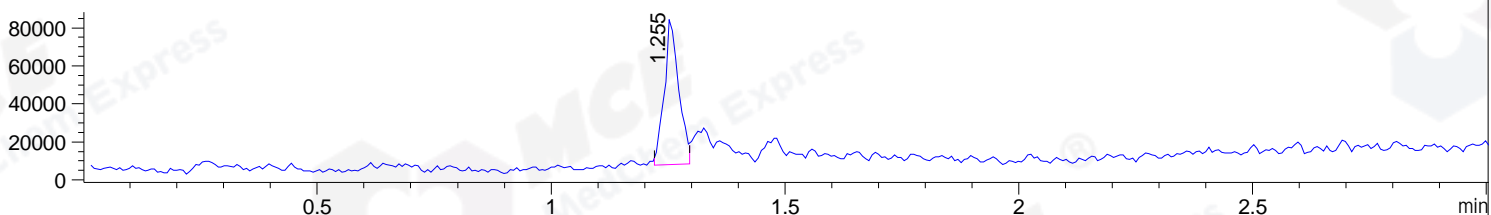

Ion 1371.6, MSD1 1371.6, Target Mass 1370.6 +H Positive, EIC=1371.3:1372.3

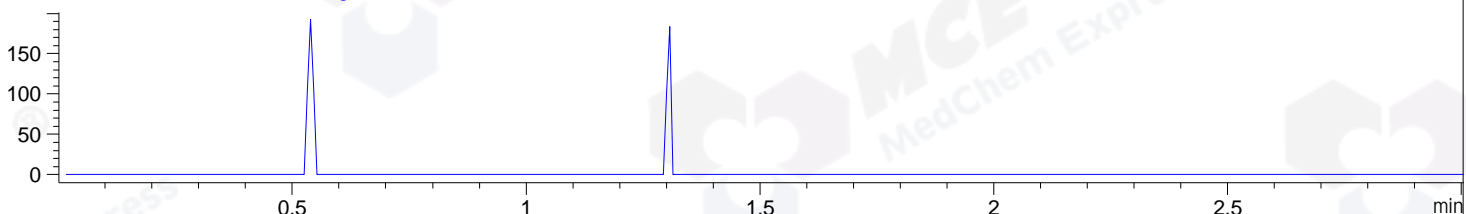

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.02	1965.53	1289.67	99.88	656
1.46	0.03	2.27	1.37	0.12	505

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.02	136.04	94.00	97.44	656
1.46	0.04	3.58	1.40	2.56	505

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.04	162677.20	78582.63	100.00	656

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

