



File ..ATA\2020\20200724\1052\BIZ2020-723-WMX10-.D Tgt Mass (CHM):  
 Injection Date : 24 Jul 20 9:52 am +0800 Seq. Line : 14  
 Sample Name : BIZ2020-723-WMX10 Location : P1-A-02  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.5 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200724\1052\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200724\1052\1-POS-3MIN.M  
 Catalog No : HY-126275  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

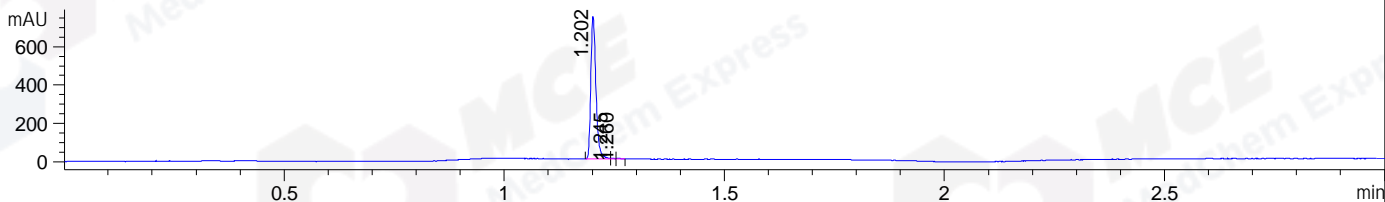


DAD1 C, Sig=254,4 Ref=off

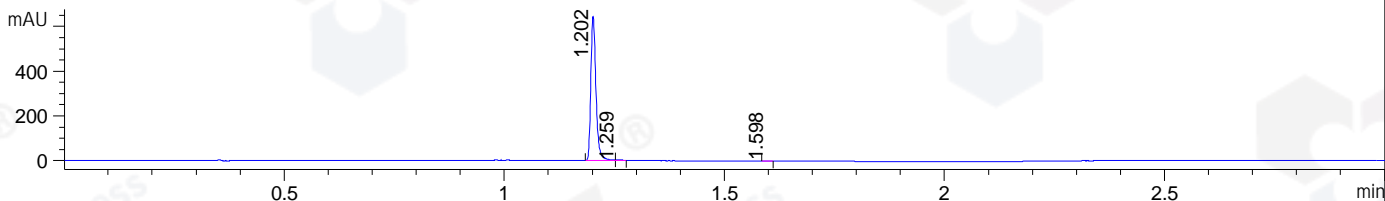

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

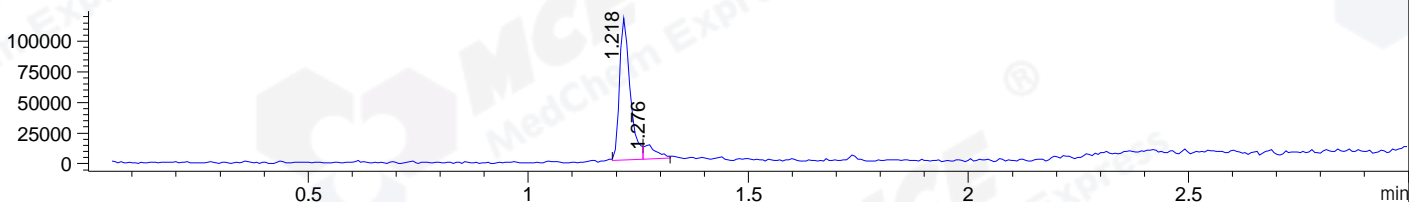

Ion 360, MSD1 360, Target Mass 359 +H Positive, EIC=359.7:360.7

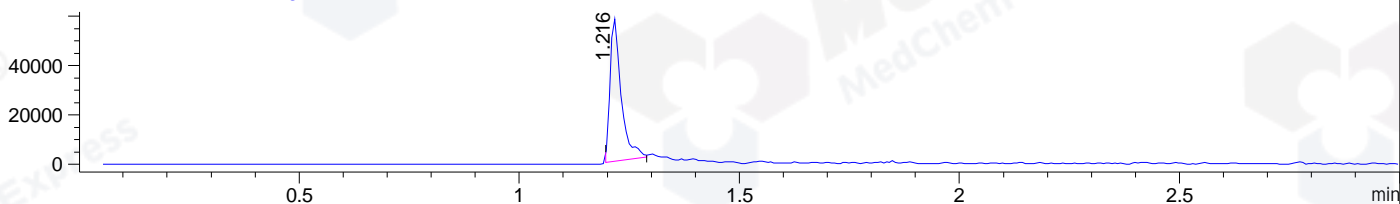

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	603.54	747.12	99.33	360
1.25	0.01	2.18	3.88	0.36	360
1.26	0.01	1.90	2.75	0.31	360

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	520.58	646.36	99.38	360
1.26	0.01	2.42	2.88	0.46	360
1.60	0.01	0.81	1.14	0.15	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.03	195070.86	117789.97	90.18	360
1.28	0.03	21248.26	11261.04	9.82	360

Ret. Time: 1.22

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.28

ES-API Positive

