
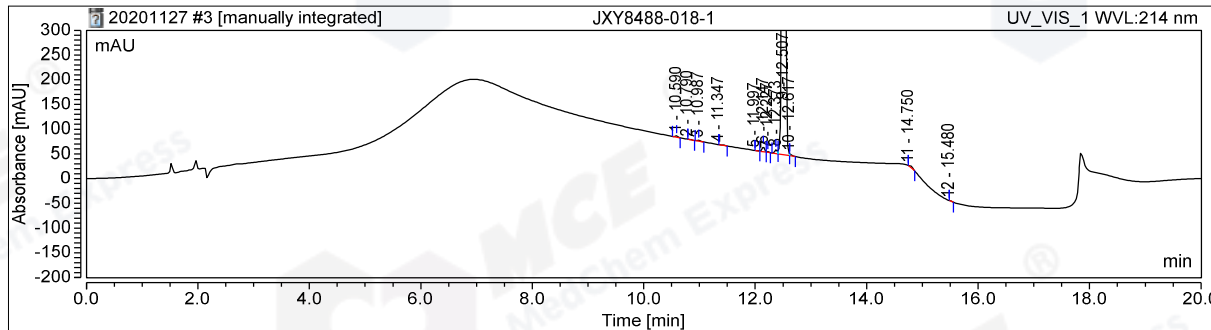


### Chromatogram and Results

#### Injection Details

<b>Injection Name:</b> JXY8488-018-1	<b>Run Time (min):</b> 20.00
<b>Vial Number:</b> GE5	<b>Injection Volume:</b> 5.00
<b>Injection Type:</b> Unknown	<b>Channel:</b> UV_VIS_1
<b>User:</b> zqq	<b>Wavelength:</b> 214
<b>Instrument Method:</b> HN-082_22-H01P01(RP-HPLC)	<b>Bandwidth:</b> 4
<b>Processing Method:</b> 3D Quantitative	<b>Dilution Factor:</b> 1.0000
<b>CAS NO.:</b> 1036969-20-6 A-RP-540	<b>Sample Weight:</b> 1.0000
<b>Injection Data/Time:</b> 27/Nov/2020 10:49	
<b>chrom://hy637/ChromeleonLocal/Instrument Data/202011/20201127.seq/367.smp/UV_VIS_1.channel/UV_VIS_1.chm</b>	

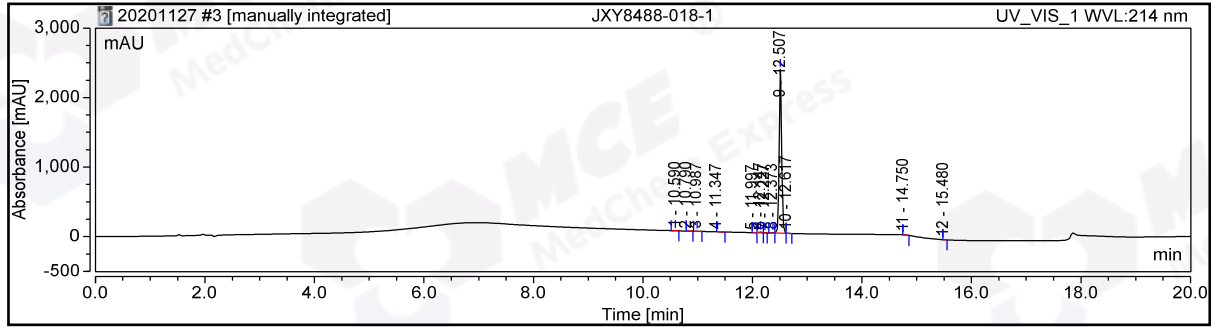

#### Integration Results

No.	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Rel.Area %
1	10.590	0.134	3.010	n.a.	998	0.10
2	10.790	0.019	0.000	n.a.	0	0.01
3	10.987	0.092	1.862	n.a.	994	0.07
4	11.347	0.038	0.000	n.a.	0	0.03
5	11.997	0.028	0.000	n.a.	0	0.02
6	12.147	0.547	11.036	1.05	999	0.42
7	12.227	0.070	1.571	n.a.	994	0.05
8	12.373	0.434	8.012	n.a.	996	0.33
9	12.507	129.447	2356.663	n.a.	999	98.68
10	12.617	0.137	3.749	n.a.	997	0.10
11	14.750	0.196	0.000	n.a.	1000	0.15
12	15.480	0.034	0.000	n.a.	1000	0.03
<b>Total:</b>	<b>131.175</b>	<b>2385.901</b>	<b>1.05</b>	<b>8977.09</b>		