



File ..DATA\2020\20200210\833\CPK2020-122-24841-.D Tgt Mass (CHM):
 Injection Date : 10 Feb 20 4:06 pm +0800 Seq. Line : 10
 Sample Name : CPK2020-122-24841 Location : P1-A-02
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2020\20200210\833\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200210\833\1-POS-3MIN.M
 Catalog No : HY-12653 Batch# 24841
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

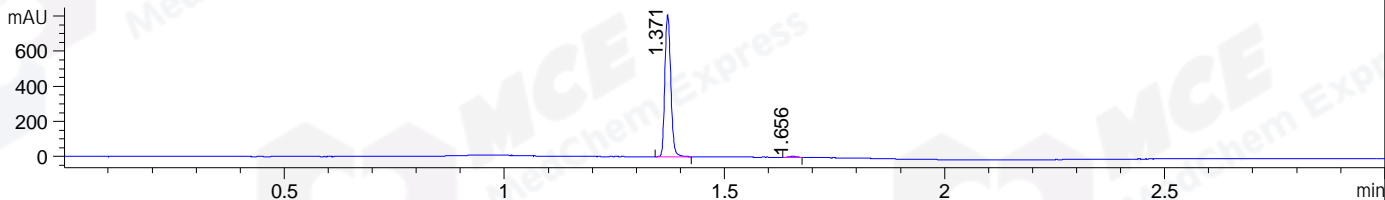


DAD1 C, Sig=254,4 Ref=off

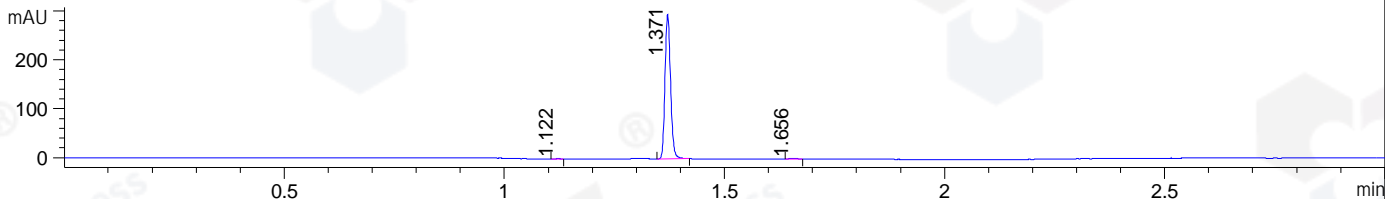

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

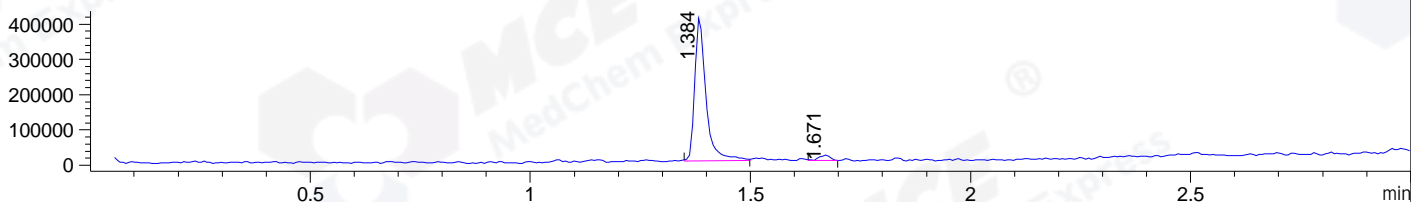

Ion 433, MSD1 433, Target Mass 432 +H Positive, EIC=432.7:433.7

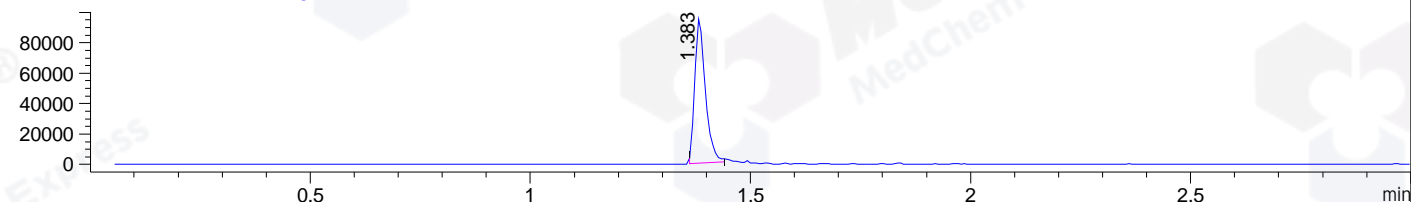

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.02	751.90	810.15	99.14	350
1.66	0.02	6.50	6.02	0.86	350

Integration Results for DAD1 C, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.01	0.97	1.29	0.37	451
1.37	0.01	257.58	295.52	99.01	350
1.66	0.02	1.61	1.61	0.62	350

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	731028.31	412206.72	96.39	350
1.67	0.03	27400.62	16225.97	3.61	350

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

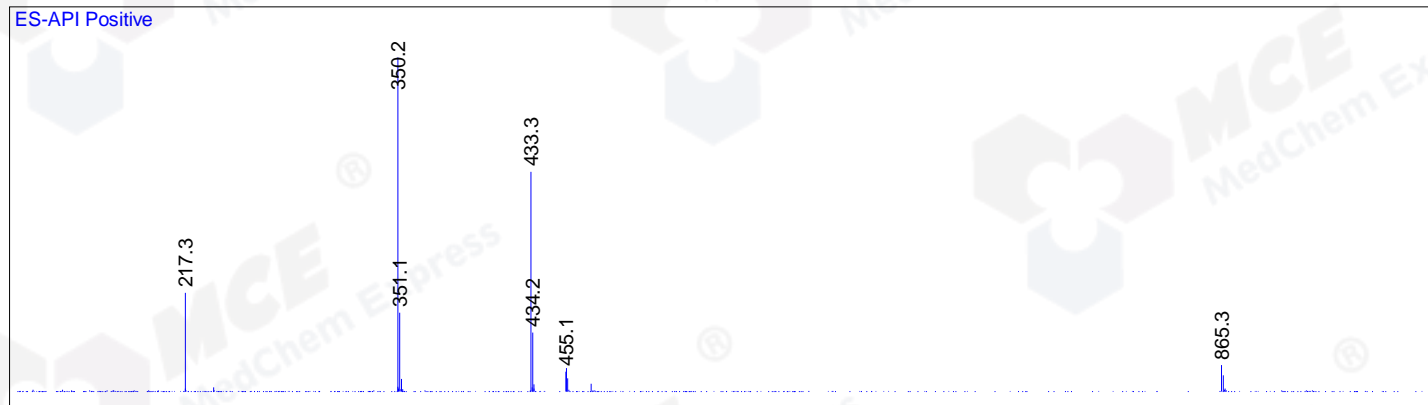

Ret. Time: 1.67

