



File ..DATA\2020\20201113\1152\CPK2020-N10-16639.D Tgt Mass (CHM):  
Injection Date : 13 Nov 20 8:11 pm +0800 Seq. Line : 121  
Sample Name : CPK2020-N10-16639 Location : P1-C-08  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20201113\1152\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20201113\1152\1-POS-3MIN.M  
Catalog No : HY-12745A  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

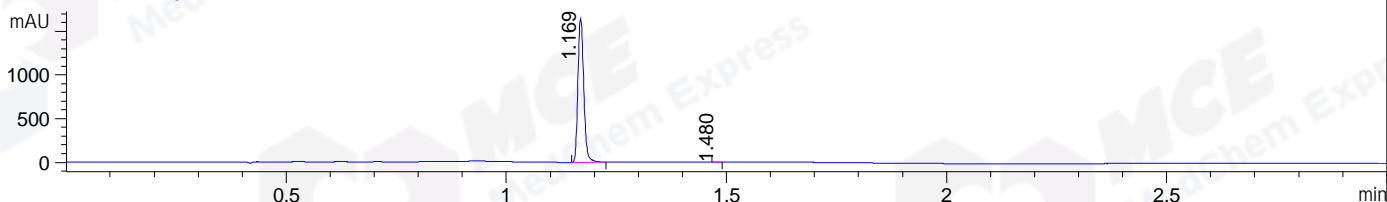


DAD1 C, Sig=254,4 Ref=off

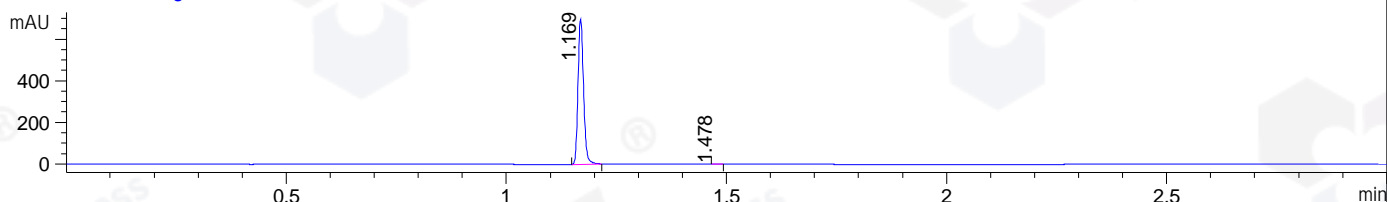

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

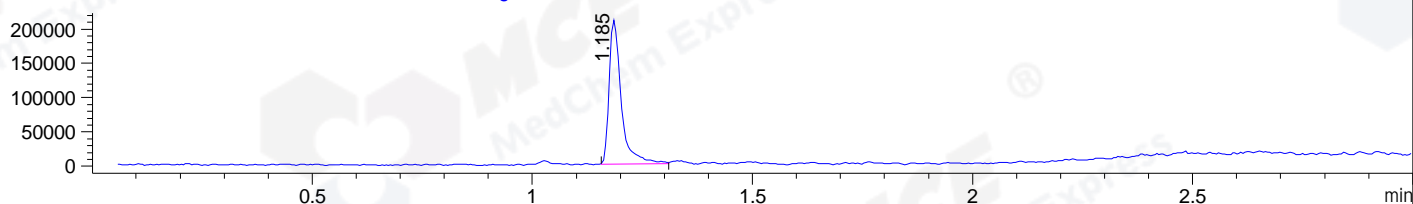

Ion 477, MSD1 477, Target Mass 476 +H Positive, EIC=476.7:477.7

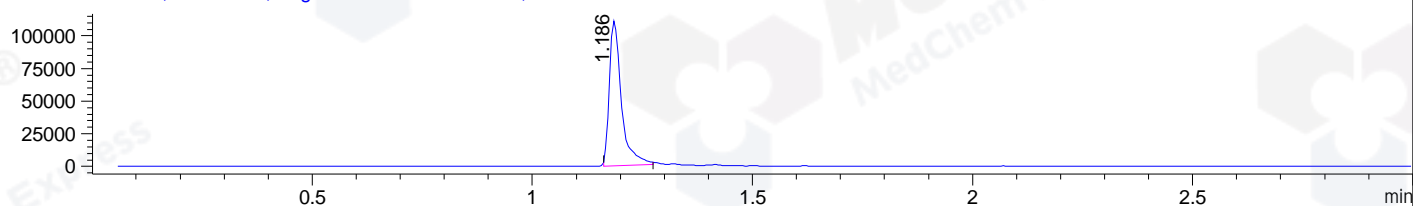

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	1513.11	1649.07	99.93	477
1.48	0.01	1.05	1.19	0.07	180

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.01	607.21	697.81	99.86	477
1.48	0.01	0.88	1.06	0.14	180

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.03	404358.38	209782.25	100.00	477

Ret. Time: 1.19

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

