



File ..DATA\2020\20200818\1075\CPK2020-817-15437.D Tgt Mass (CHM):  
Injection Date : 18 Aug 20 10:50 pm +0800 Seq. Line : 70  
Sample Name : CPK2020-817-15437 Location : P1-C-03  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200818\1075\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200818\1075\1-POS-3MIN.M  
Catalog No : HY-12755  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

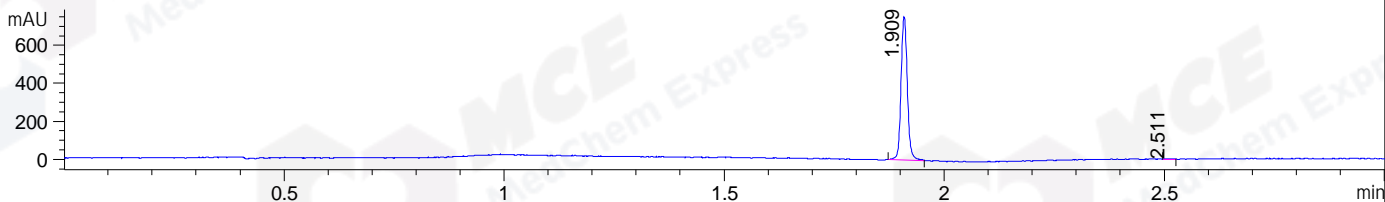


DAD1 C, Sig=254,4 Ref=off

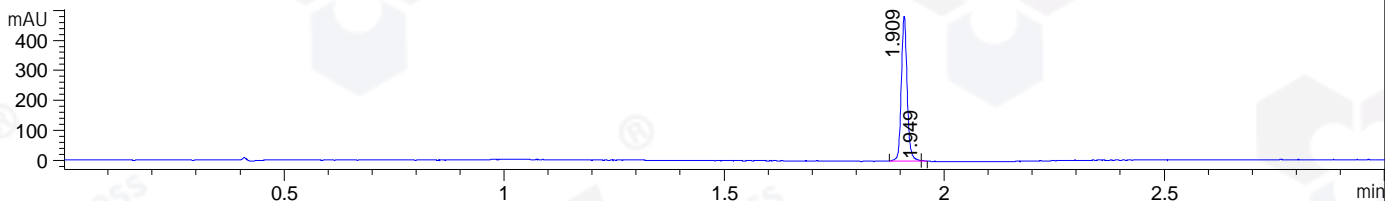

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

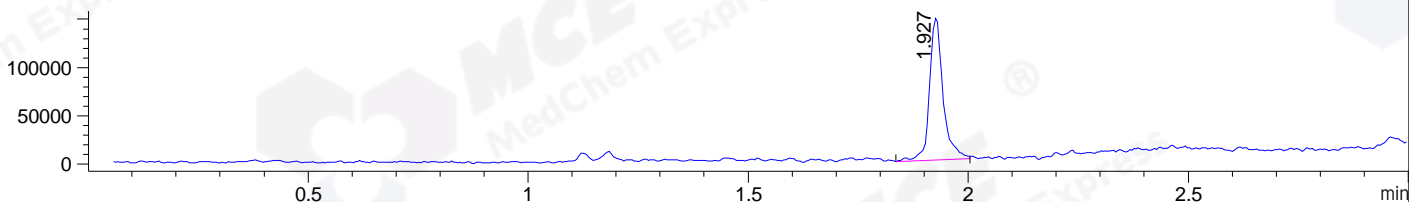

Ion 408, MSD1 408, Target Mass 407 +H Positive, EIC=407.7:408.7

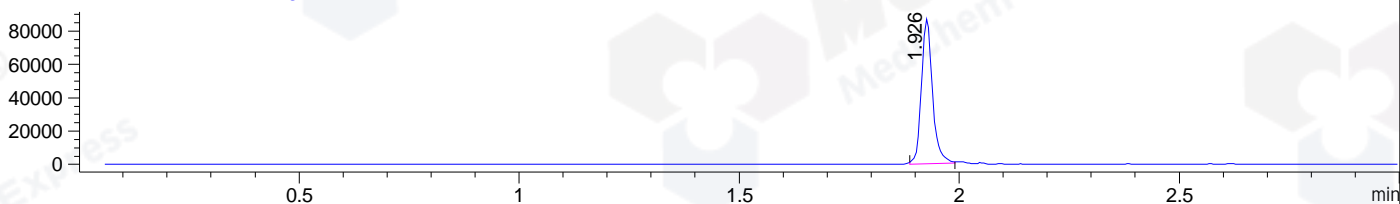

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.91	0.02	750.68	755.39	99.53	408
2.51	0.02	3.57	2.91	0.47	253

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.91	0.02	444.85	483.34	99.71	408
1.95	0.01	1.31	3.08	0.29	408

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.93	0.03	316120.16	147006.34	100.00	408

Ret. Time: 1.93

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

