



File ..\DATA\2020\20200330\902\CPK2020-324-25635.D Tgt Mass (CHM):  
 Injection Date : 30 Mar 20 10:36 am +0800 Seq. Line : 19  
 Sample Name : CPK2020-324-25635 Location : P1-A-04  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200330\902\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200330\902\1-POS-3MIN.M  
 Catalog No : HY-12762 Batch#25635  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

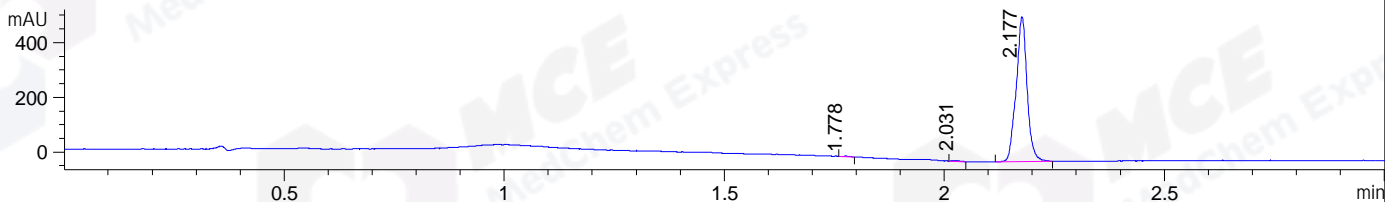


DAD1 C, Sig=254,4 Ref=off

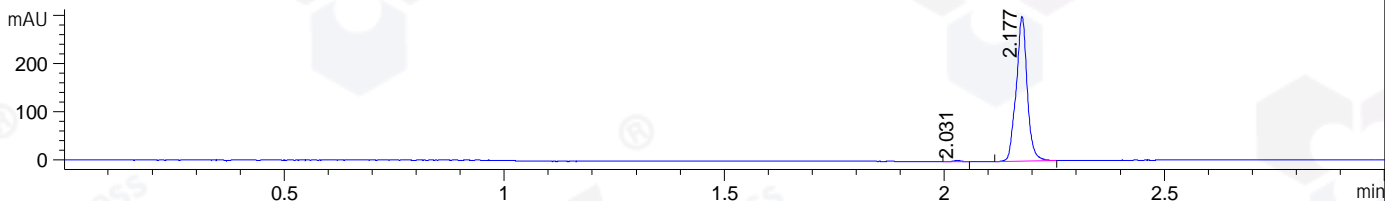

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

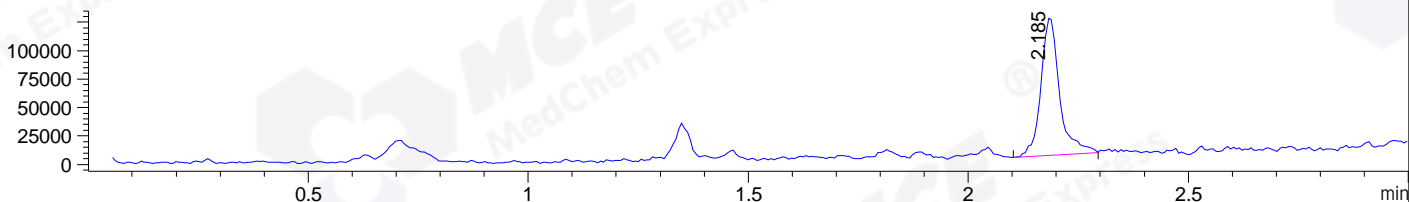

Ion 568, MSD1 568, Target Mass 567 +H Positive, EIC=567.7:568.7

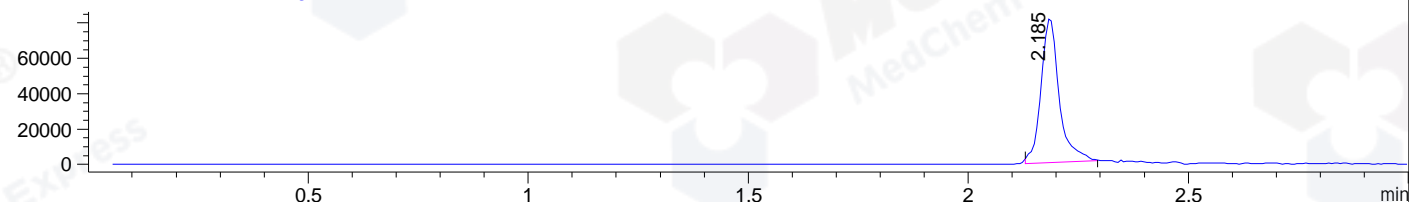

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.78	0.02	2.07	2.19	0.22	ND
2.03	0.02	3.29	3.00	0.36	470
2.18	0.03	915.27	530.49	99.42	568

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.03	0.02	3.49	2.61	0.67	470
2.18	0.03	521.01	300.22	99.33	568

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.19	0.04	360715.38	122236.57	100.00	568

Ret. Time: 2.19

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

570.3

569.3

568.3