



File ..\DATA\2019\20190716\630\CPK2019-715-22452.D Tgt Mass (CHM):
 Injection Date : 16 Jul 19 3:22 pm +0800 Seq. Line : 82
 Sample Name : CPK2019-715-22452 Location : P1-B-05
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190716\630\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190716\630\1-POS-3MIN.M
 Catalog No : HY-12795 Batch#22452
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

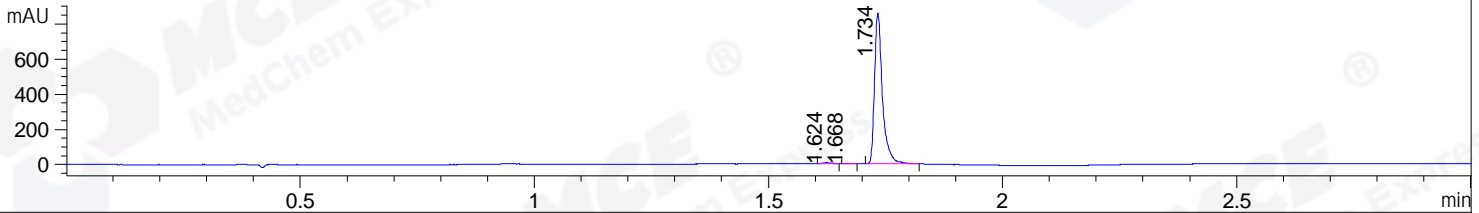


DAD1 C, Sig=254,4 Ref=off

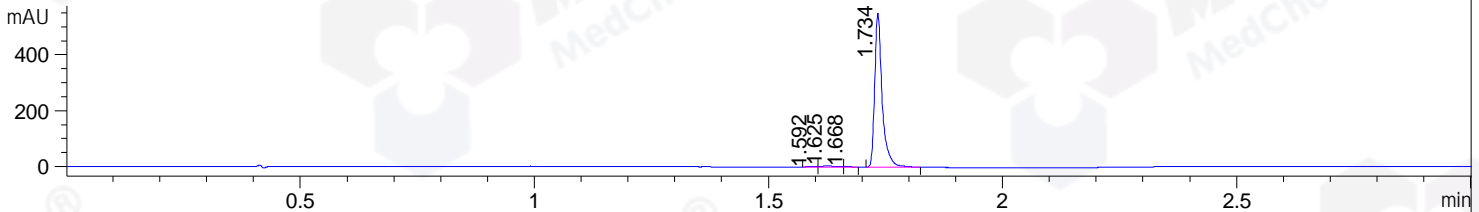

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

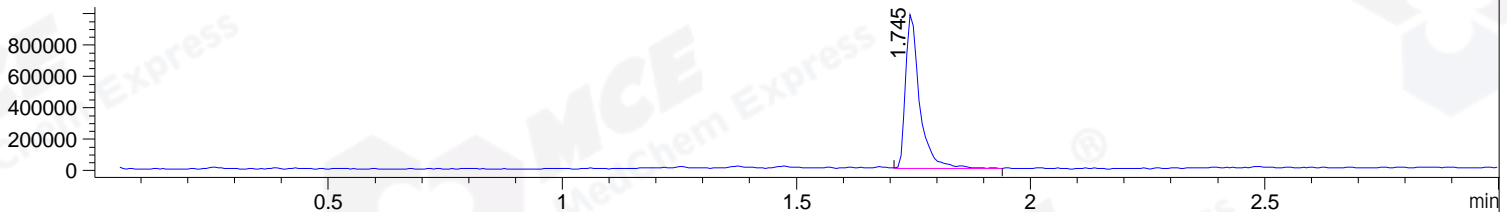

Ion 426.9247, MSD1 426.9247, Target Mass 425.9247 +H Positive, EIC=426.62:427.62

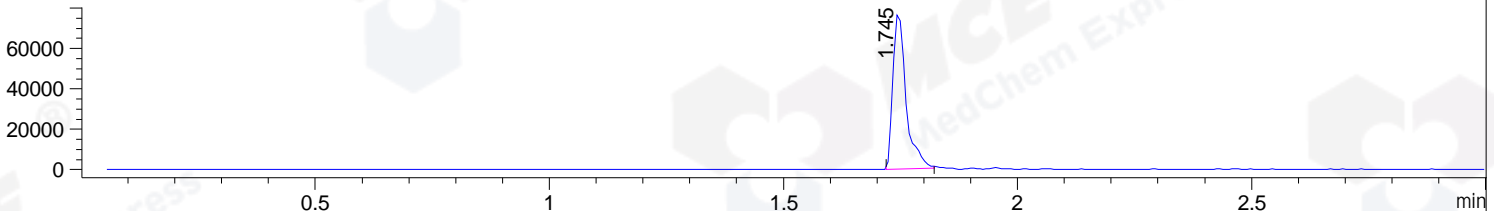

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.62	0.02	6.53	5.56	0.64	ND
1.67	0.01	1.45	1.68	0.14	412
1.73	0.02	1008.50	859.55	99.22	426

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.59	0.02	1.43	1.18	0.23	ND
1.63	0.03	6.77	3.93	1.09	ND
1.67	0.01	1.28	1.46	0.21	412
1.73	0.02	610.27	551.38	98.47	426

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.74	0.03	2077291.13	995476.56	100.00	426

Ret. Time: 1.74

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

