



Chromatogram and Results

Injection Details

Injection Name:	WGY7769-003-6	Injection Volume:	3.00
Vial Number:	BA2	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	224
Calibration Level:		Users:	ghj
Instrument Method:	LD862_1-H01P01(RP-HPLC)	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	17/Apr/20 12:08	Run Time (min):	16.00
Comment:	LD862_1-20200417 A-RP-521		

chrom://hy261/Themo/Instrument Data/202004/20200417.seq/645.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

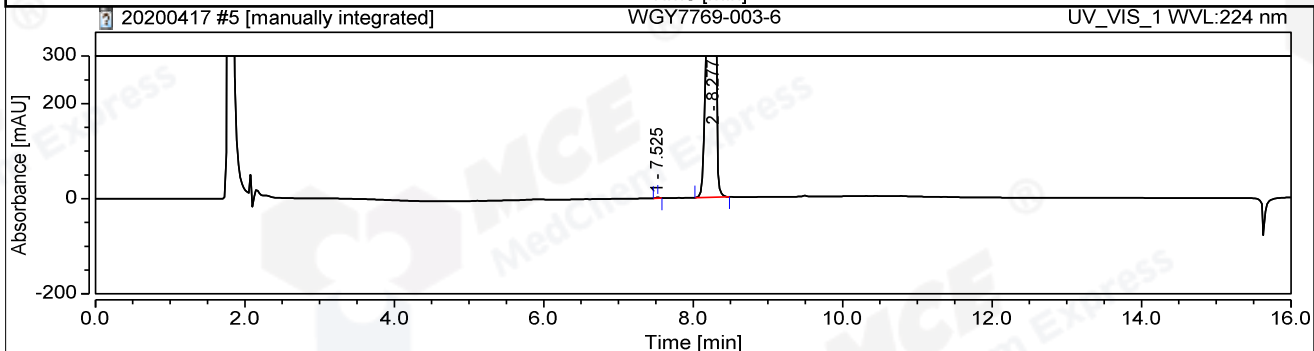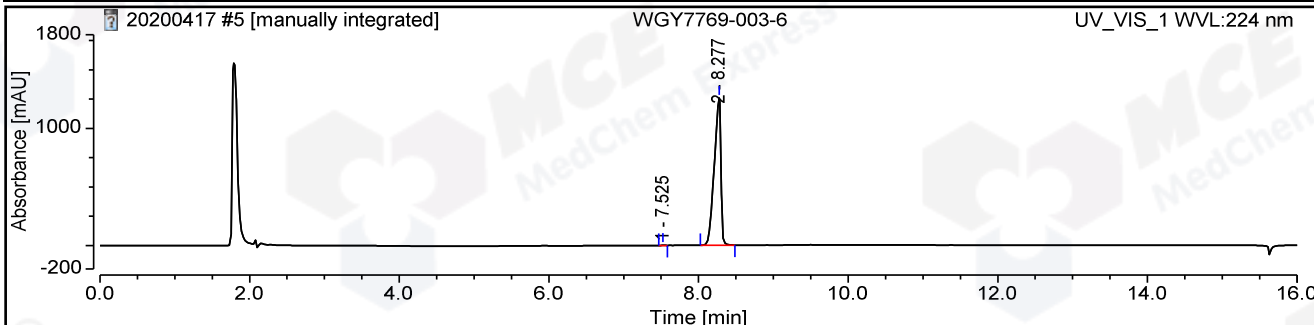

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		7.525	0.102	2.520	0.96	6.44	0.08
2		8.277	131.359	1256.035	0.68	n.a.	99.92
Total:			131.462	1258.555	1.64	6.44	



Chromatogram and Results

Injection Details

Injection Name:	BLANK	Injection Volume:	5.00
Vial Number:	BA1	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	224
Calibration Level:		Users:	ghj
Instrument Method:	LD862_1-H01P01(RP-HPLC)	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	17/Apr/20 11:20	Run Time (min):	16.00
Comment:	LD862_1-BLANK A-RP-521		

chrom://hy261/Themo/Instrument Data/202004/20200417.seq/428.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

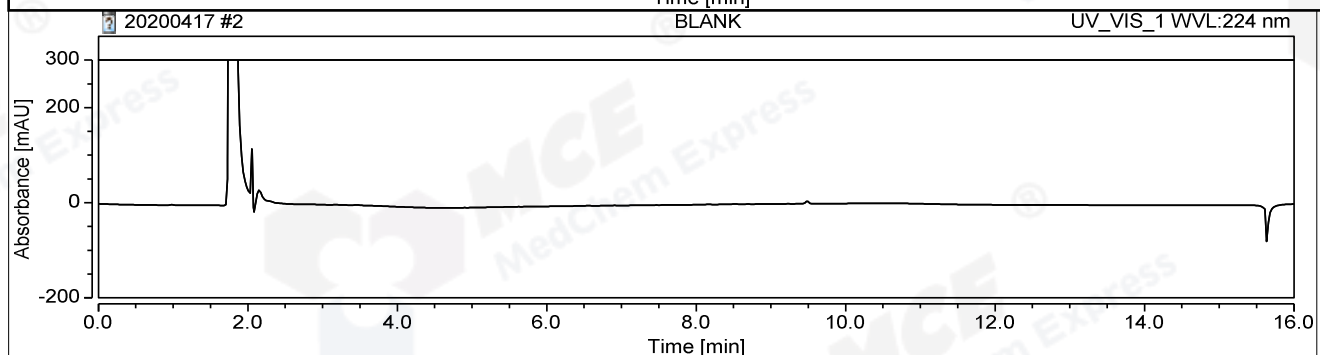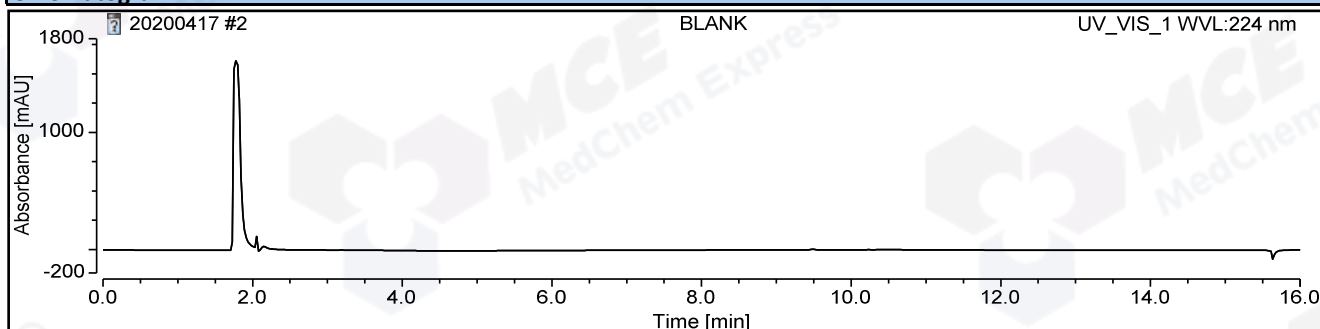

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
Total:			0.000	0.000	0.00	0.00	