


**21 BIZ2019-923-CXL6****Catalog No: HY-128695 Batch#46133 A-RP-243 JLW**

Sample Name:	<b>BIZ2019-923-CXL6</b>	Injection Volume:	<b>2.0</b>
Vial Number:	<b>GB3</b>	Channel:	<b>UV_VIS_1</b>
Sample Type:	<b>unknown</b>	Wavelength:	<b>214</b>
Control Program:	<b>10-90A 214NM</b>	Bandwidth:	<b>n.a.</b>
Quantif. Method:	<b>default</b>	Dilution Factor:	<b>1.0000</b>
Recording Time:	<b>2019-9-24 22:10</b>	Sample Weight:	<b>1.0000</b>
Run Time (min):	<b>16.00</b>	Sample Amount:	<b>1.0000</b>

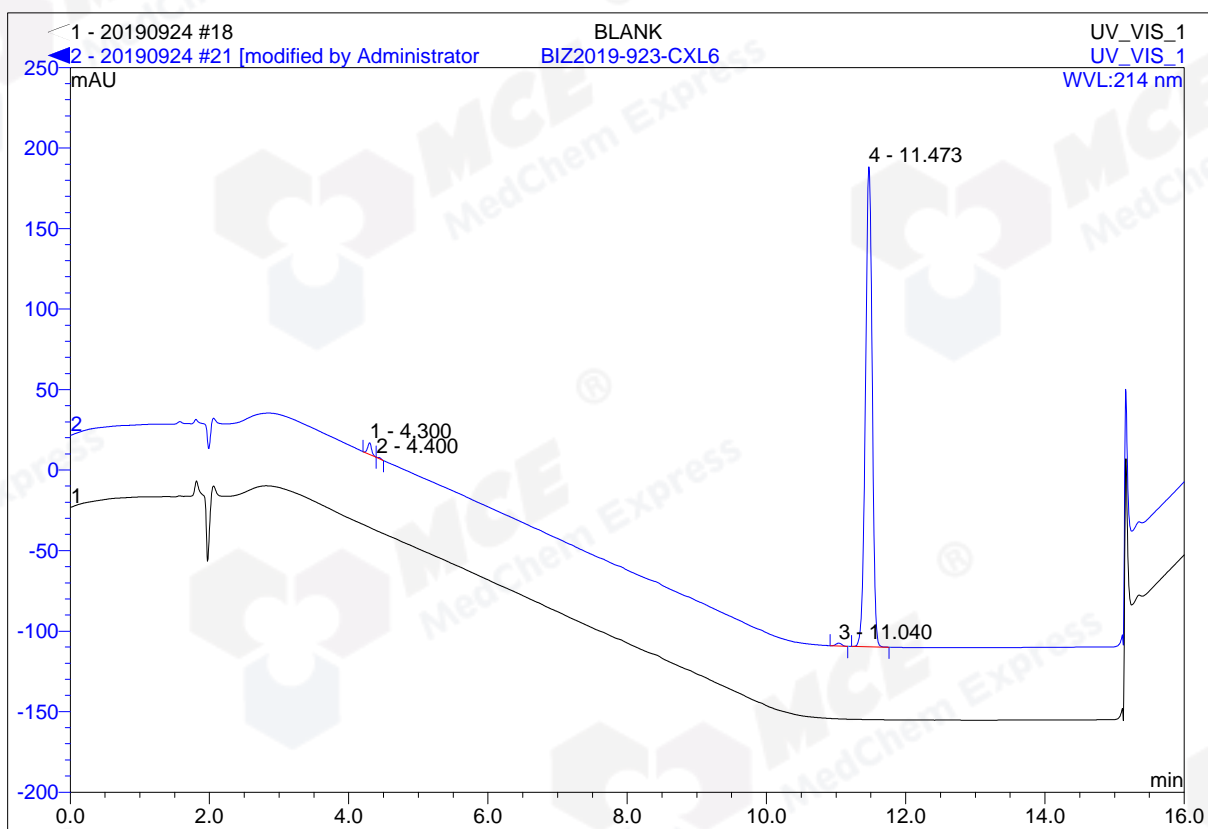

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	4.30	n.a.	7.227	0.459	1.35	n.a.	BMB*
2	4.40	n.a.	0.016	0.034	0.10	n.a.	bMB*
3	11.04	n.a.	1.817	0.170	0.50	n.a.	BMB
4	11.47	n.a.	298.108	33.292	98.05	n.a.	BMB
<b>Total:</b>			307.169	33.955	100.00	0.000	