
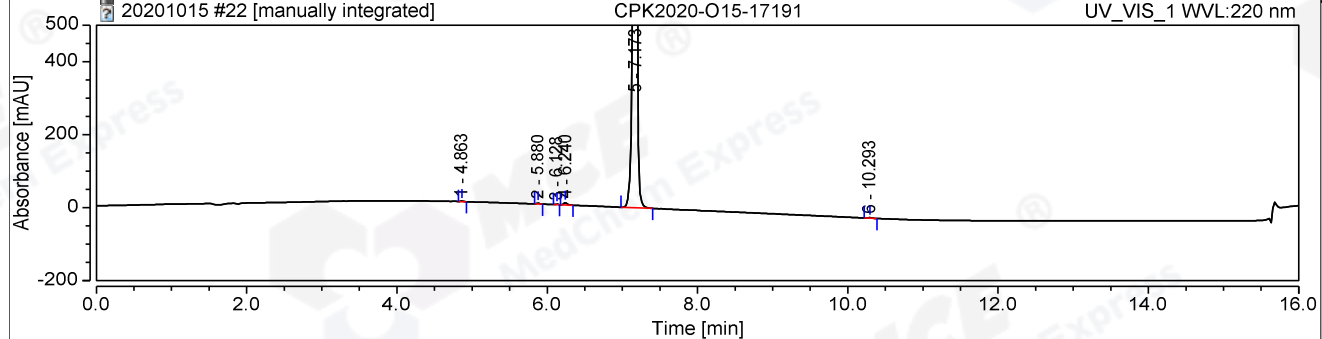


Chromatogram and Results

| Injection Details | | | |
|---|-----------------------------|-------------------|----------|
| Injection Name: | CPK2020-O15-17191 | Injection Volume: | 2.00 |
| Vial Number: | GD3 | Channel: | UV_VIS_1 |
| Injection Type: | Unknown | Wavelength: | 220 |
| Calibration Level: | | Users: | jlw |
| Instrument Method: | 30-90A,220NM | Dilution Factor: | 1.0000 |
| Processing Method: | New Processing Method | Sample Weight: | 1.0000 |
| Injection Date/Time: | 15/Oct/20 18:22 | Run Time (min): | 16.00 |
| Comment: | HM-411_11-20201015 A-RP-540 | | |
| chrom://hy261/Themo/Instrument Data/202010/20201015.seq/563.smp/UV_VIS_1.channel/UV_VIS_1.chm | | | |

Chromatogram

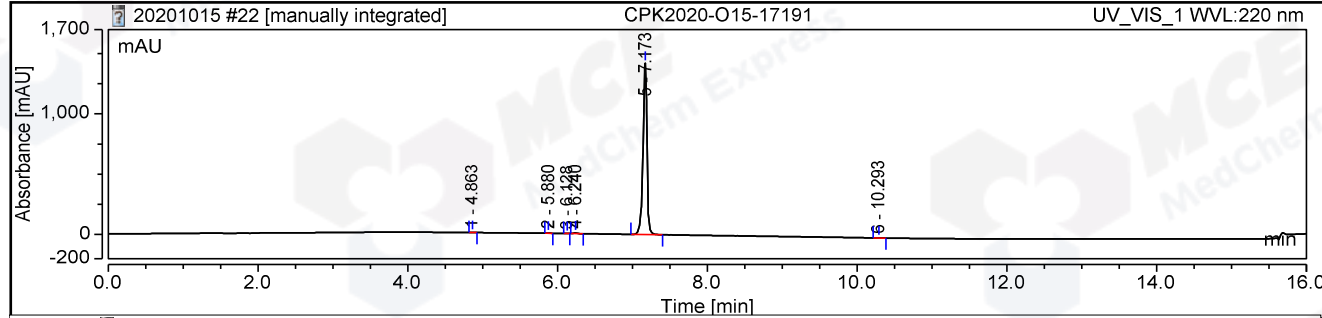

| Integration Results | | | | | | | |
|---------------------|-----------|-----------------------|-----------------|---------------|----------------|---------|---------------|
| No. | Peak Name | Retention Time min | Area mAU*min | Height mAU | Asymmetry (EP) | S/N | Rel.Area % |
| 1 | | 4.863 | 0.072 | 1.832 | 1.08 | 9.3 | 0.08 |
| 2 | | 5.880 | 0.105 | 2.625 | 1.11 | 13.3 | 0.12 |
| 3 | | 6.128 | 0.040 | 1.101 | 0.97 | 5.6 | 0.05 |
| 4 | | 6.240 | 0.328 | 6.761 | 1.17 | 34.2 | 0.37 |
| 5 | | 7.173 | 87.297 | 1420.658 | 0.83 | 7192.6 | 99.28 |
| 6 | | 10.293 | 0.084 | 1.710 | 0.93 | 8.7 | 0.10 |
| Total: | | | 87.926 | 1434.687 | 6.09 | 7263.64 | |