



File ..\DATA\2020\20200922\1113\BIZ2020-921-SCH5.D Tgt Mass (CHM):
 Injection Date : 22 Sep 20 2:20 pm +0800 Seq. Line : 62
 Sample Name : BIZ2020-921-SCH5 Location : P1-A-08
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200922\1113\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200922\1113\1-POS-3MIN.M
 Catalog No : HY-128773A
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

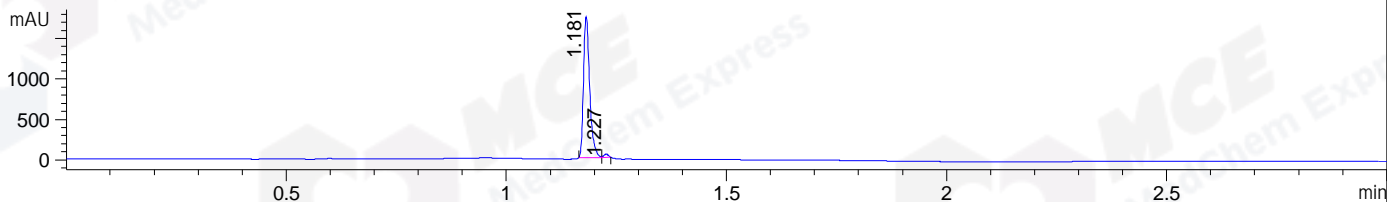


DAD1 C, Sig=254,4 Ref=off

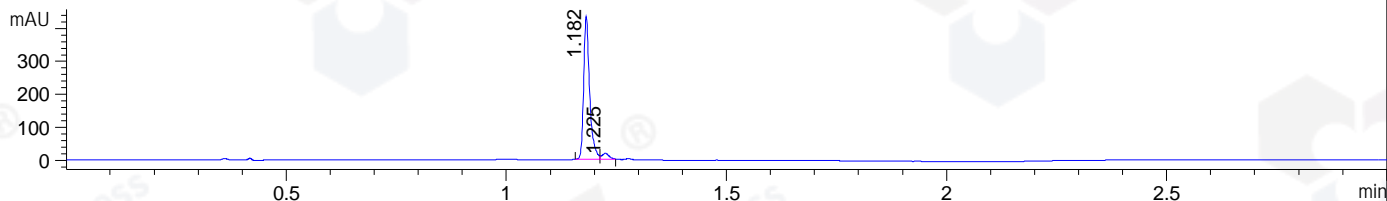

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

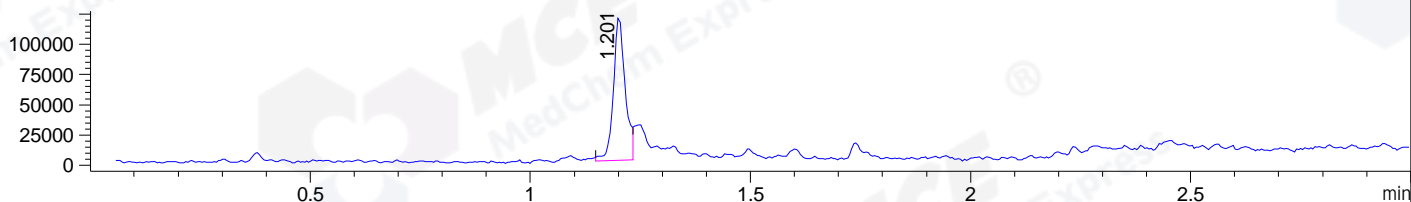

Ion 623, MSD1 623, Target Mass 622 +H Positive, EIC=622.7:623.7

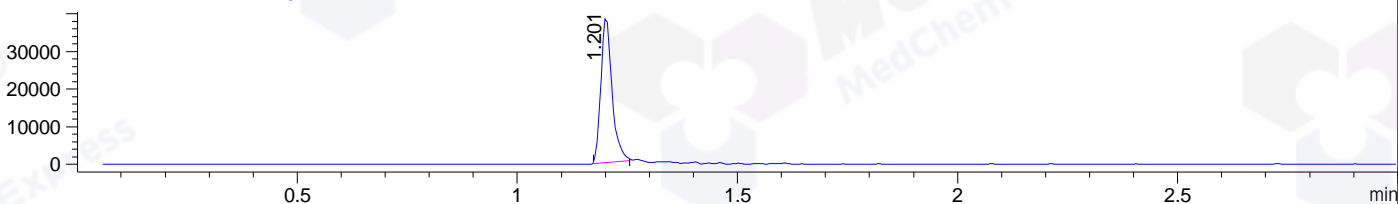

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.18	0.02	1702.59	1746.43	98.36	312
1.23	0.01	28.47	40.12	1.64	623

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.18	0.02	409.50	434.32	95.58	312
1.23	0.02	18.92	17.75	4.42	623

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.03	220036.55	118430.82	100.00	312

Ret. Time: 1.20

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

