



Chromatogram and Results

Injection Details

Injection Name:	ZGZS8415-005-2	Injection Volume:	5.00
Vial Number:	RA7	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	210
Calibration Level:		Users:	jlw
Instrument Method:	HM-713L_2-H01P02(RP-HPLC)	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	27/Oct/20 14:54	Run Time (min):	25.00
Comment:	HM-713L_2-20201026 A-RP-425		

chrom://hy261/Themo/Instrument Data/202010/20201027.seq/622.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

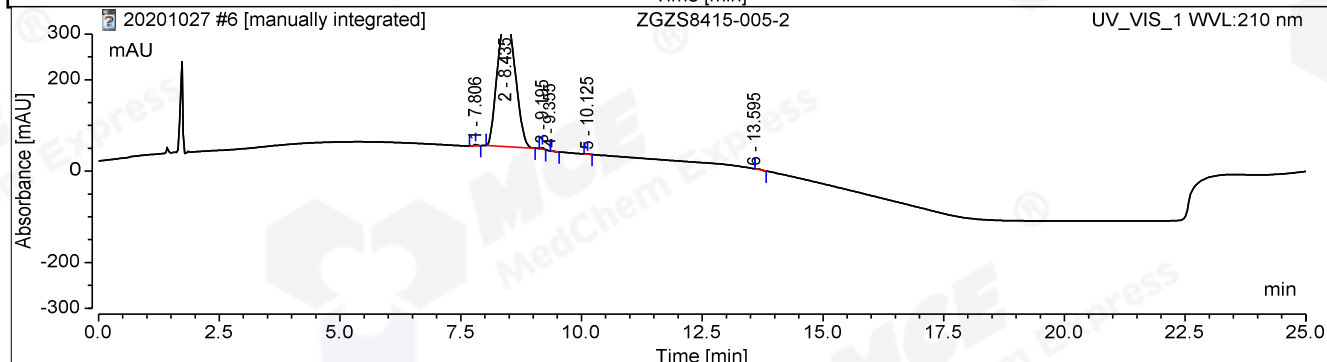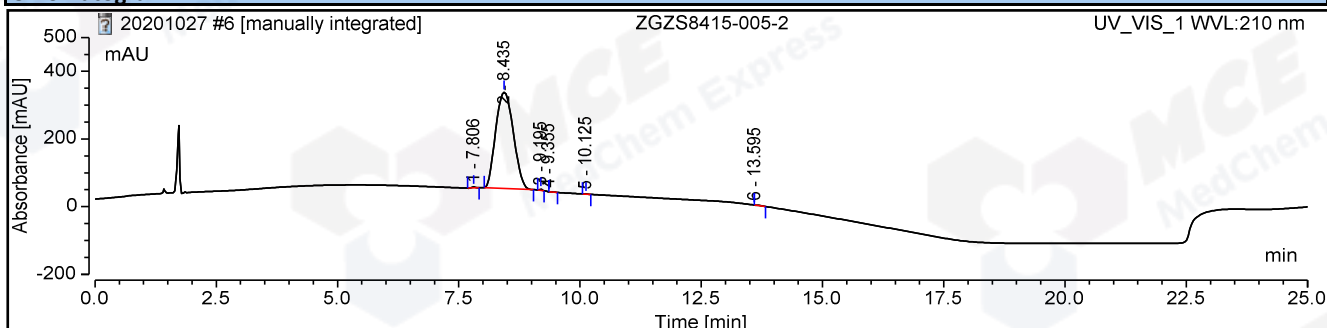

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	S/N	Rel.Area %
1		7.806	0.242	3.251	1.14	14.3	0.20
2		8.435	120.037	284.284	1.12	1247.4	99.48
3		9.195	0.211	3.479	1.02	15.3	0.18
4		9.355	0.026	0.000	n.a.	0.0	0.02
5		10.125	0.054	0.779	1.28	3.4	0.04
6		13.595	0.099	0.000	n.a.	0.0	0.08
Total:			120.670	291.793	4.56	1280.38	