



File ..DATA\2020\20201103\1143\CPK2020-N03-17532.D Tgt Mass (CHM):  
 Injection Date : 3 Nov 20 8:04 pm +0800 Seq. Line : 125  
 Sample Name : CPK2020-N03-17532 Location : P1-E-01  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20201103\1143\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20201103\1143\1-POS-3MIN.M  
 Catalog No : HY-12990  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

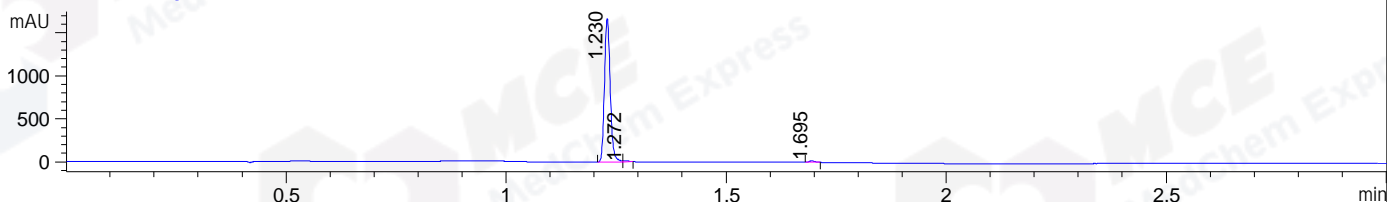


DAD1 C, Sig=254,4 Ref=off

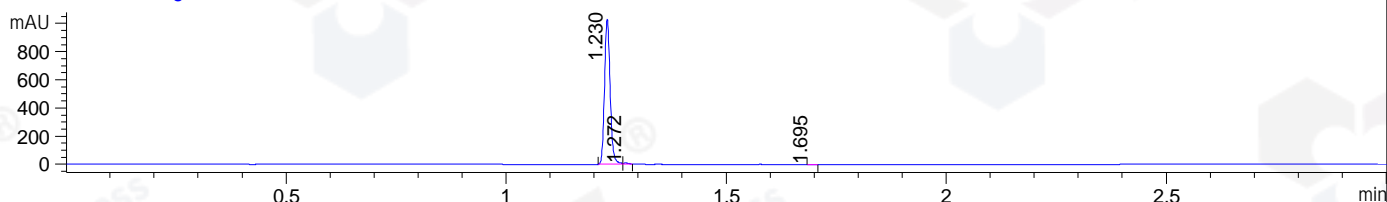

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

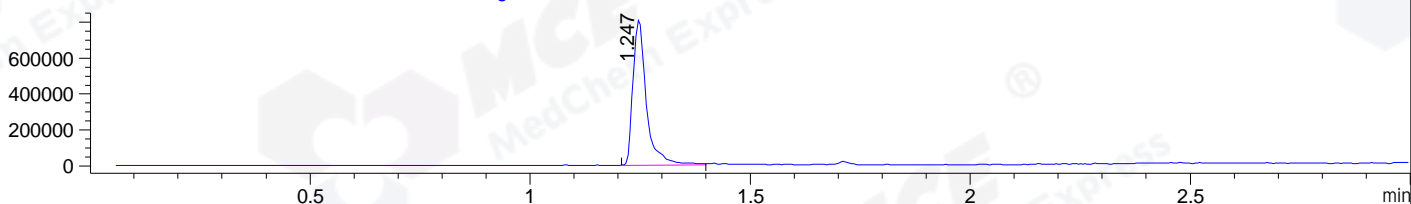

Ion 272, MSD1 272, Target Mass 271 +H Positive, EIC=271.7:272.7

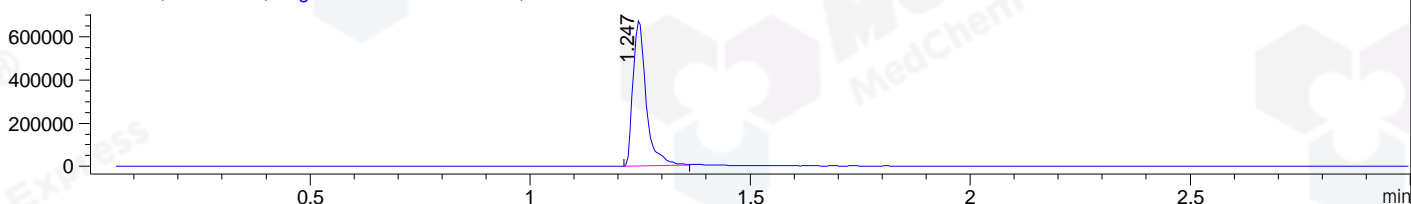

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.02	1507.99	1667.05	98.43	272
1.27	0.01	10.01	12.12	0.65	272
1.69	0.01	14.02	16.10	0.92	277

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.01	907.65	1030.15	99.26	272
1.27	0.01	6.03	7.29	0.66	272
1.69	0.01	0.77	1.03	0.08	277

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.03	1718712.25	811643.75	100.00	272

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

272.1

273.1