



File ..DATA\2020\20201026\1136\CPK2020-O21-29011.D Tgt Mass (CHM):
Injection Date : 26 Oct 20 1:25 pm +0800 Seq. Line : 47
Sample Name : CPK2020-O21-29011 Location : P1-B-07
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201026\1136\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201026\1136\1-POS-3MIN.M
CAS NO. : 849217-68-1
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

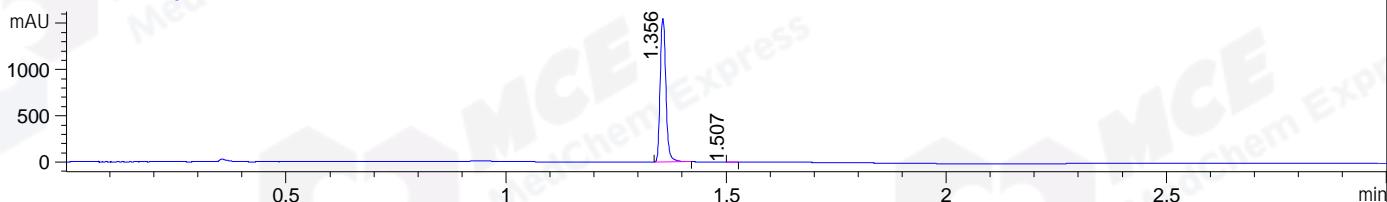


DAD1 C, Sig=254,4 Ref=off

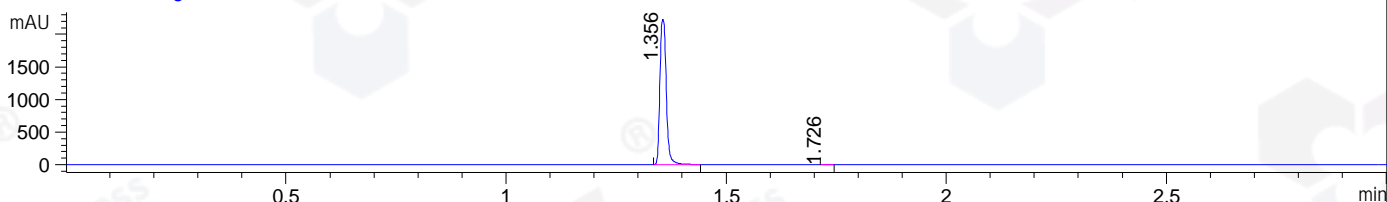

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

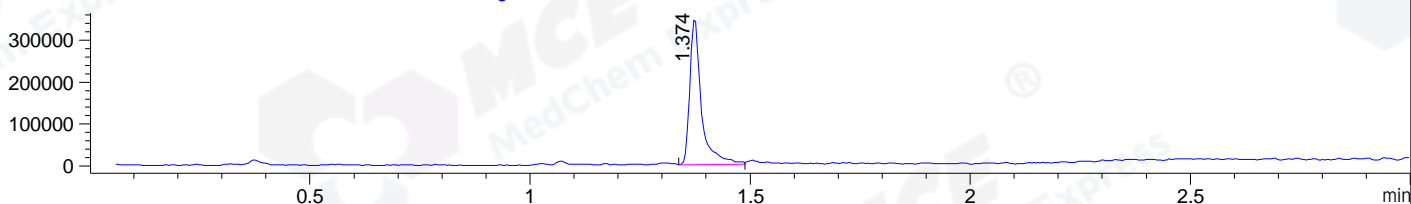

Ion 502, MSD1 502, Target Mass 501 +H Positive, EIC=501.7:502.7

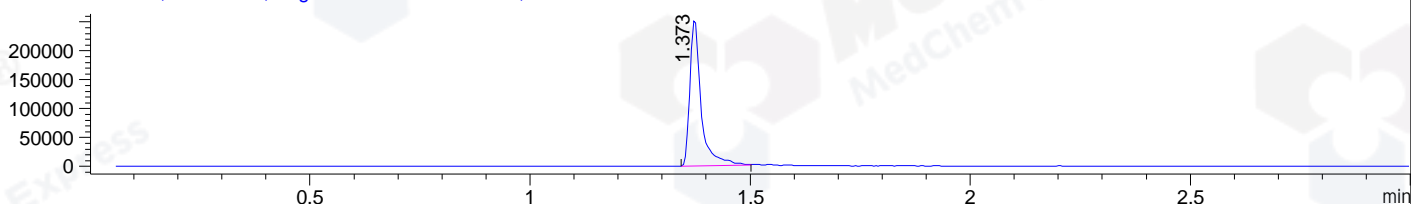

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	1409.62	1551.20	99.96	502
1.51	0.02	0.50	0.51	0.04	502

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	2236.55	2231.18	99.94	502
1.73	0.01	1.42	1.68	0.06	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.03	638337.25	351118.19	100.00	502

Ret. Time: 1.37

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

