



File ..\DATA\2020\20200222\844\CPK2020-219-05975.D Tgt Mass (CHM):
 Injection Date : 22 Feb 20 11:53 am +0800 Seq. Line : 39
 Sample Name : CPK2020-219-05975 Location : P1-B-02
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200222\844\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200222\844\1-POS-3MIN.M
 Catalog No : HY-13020 Batch# 05975
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

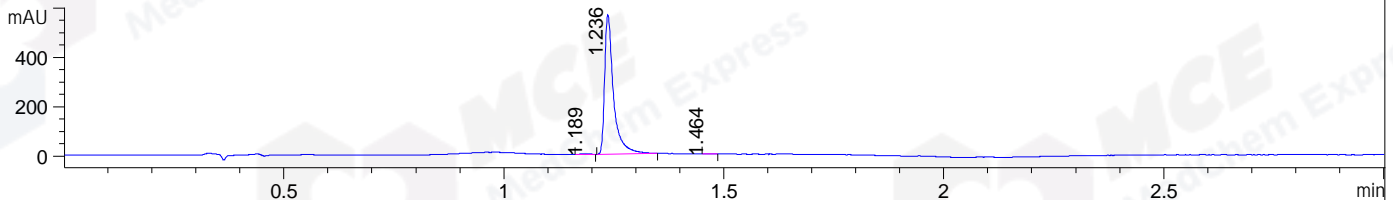


DAD1 C, Sig=254,4 Ref=off

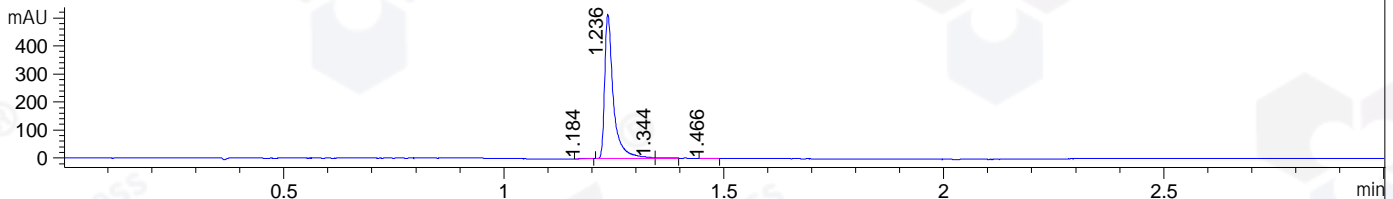

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

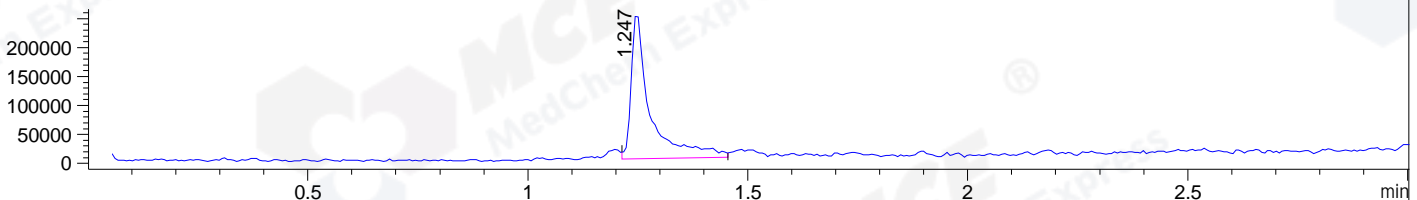

Ion 533, MSD1 533, Target Mass 532 +H Positive, EIC=532.7:533.7

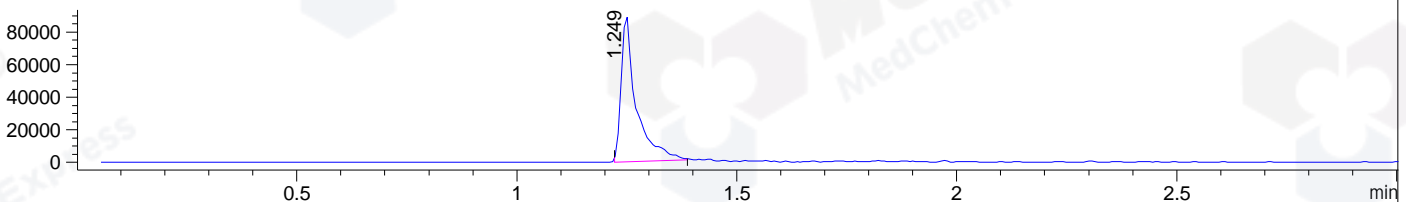

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.03	3.97	2.51	0.50	308
1.24	0.02	793.64	566.58	99.28	267
1.46	0.02	1.77	1.66	0.22	446

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.18	0.02	1.64	1.42	0.23	308
1.24	0.02	708.47	515.25	98.87	267
1.34	0.03	4.24	2.52	0.59	533
1.47	0.03	2.20	1.46	0.31	446

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.04	747078.06	254985.14	100.00	267

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

