


File ..\DATA\2020\20200417\925\BIZ2020-417-SCH2-.D Tgt Mass (CHM):
 Injection Date : 17 Apr 20 3:06 pm +0800 Seq. Line : 79
 Sample Name : BIZ2020-417-SCH2 Location : P1-A-02
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\Chem32\1\data\2020\20200417\925\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200417\925\1-POS-3MIN.M
 Catalog No : HY-13038A Batch#63058
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45

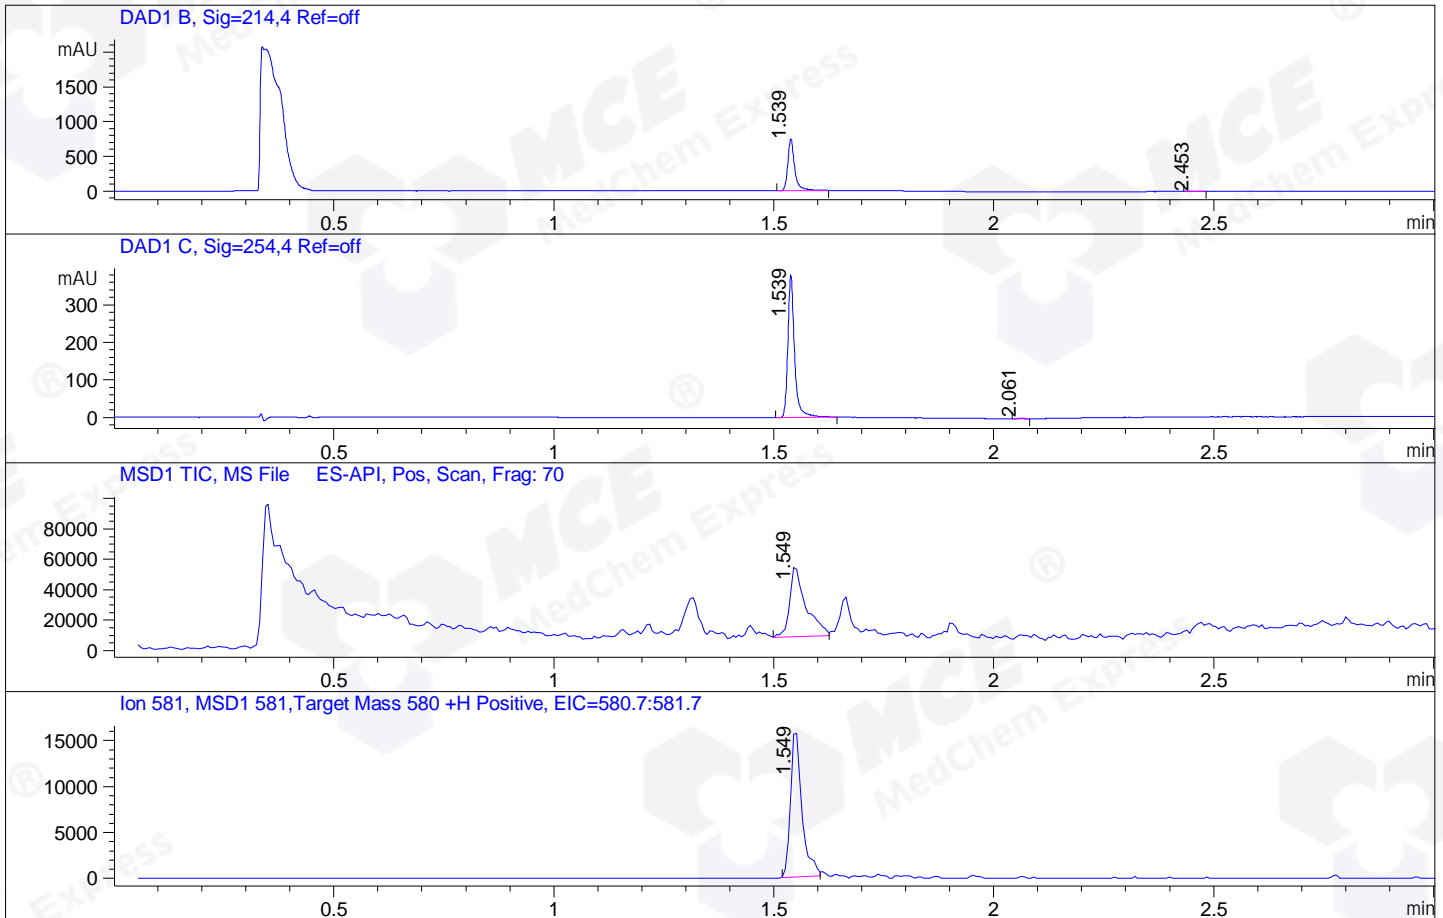

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.54	0.02	813.43	749.70	99.20	565
2.45	0.02	6.56	5.52	0.80	157

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.54	0.02	405.85	380.11	99.68	565
2.06	0.02	1.30	1.32	0.32	157

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.55	0.04	118708.57	46781.94	100.00	565

Ret. Time: 1.55

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

