



Chromatogram and Results

Injection Details

Injection Name: CJM7849-030-02	Injection Volume: 5.00
Vial Number: RC3	Channel: UV_VIS_1
Injection Type: Unknown	Wavelength: 272
Calibration Level:	Users: sy
Instrument Method: HY-003_VD3_IPF-H01P01(RP-HPLC)	Dilution Factor: 1.0000
Processing Method: New Processing Method	Sample Weight: 1.0000
Injection Date/Time: 12/Jun/20 16:21	Run Time (min): 20.00
Comment: HY-003_VD3_IPF-20200611B A-RP-538	

chrom://hy261/Themo/HY-003/HY-003_VD3/202006/20200612.seq/531.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

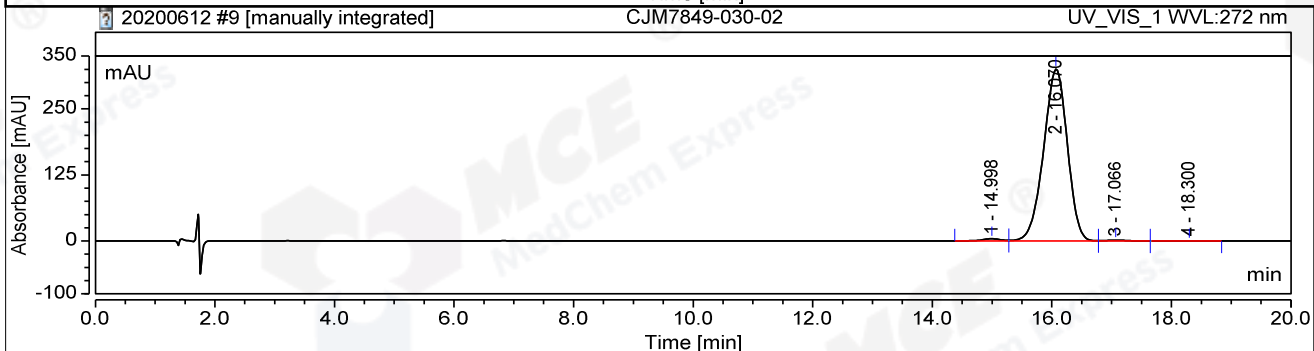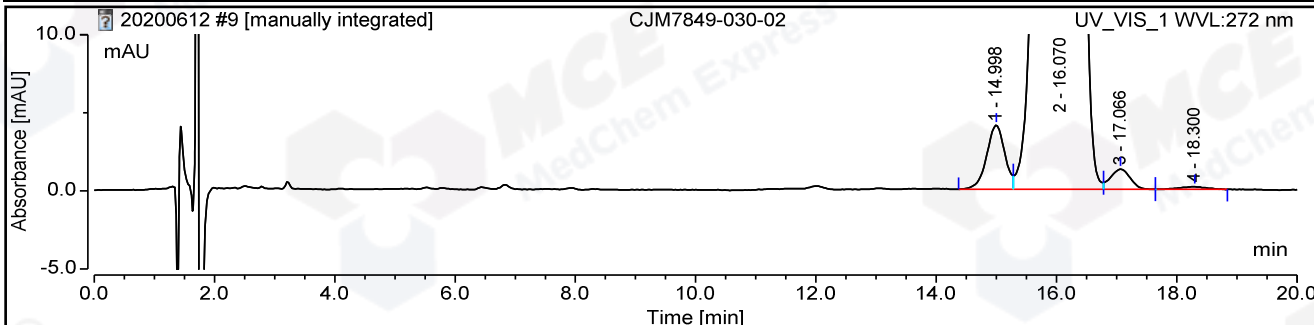

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		14.998	1.431	4.108	n.a.	1.69	0.94
2		16.070	149.707	325.374	0.94	1.47	98.68
3		17.066	0.494	1.303	n.a.	1.86	0.33
4		18.300	0.083	0.178	0.93	n.a.	0.05
Total:			151.715	330.963	1.87	5.02	