

File ..\DATA\2020\20200513\957\BIZ2020-511-SCH12.D Tgt Mass (CHM):

Injection Date : 13 May 20 5:36 pm +0800 Seq. Line : 42

Sample Name : BIZ2020-511-SCH12 Location : P1-A-05

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.5 ul

Acq. Method : D:\Chem32\1\data\2020\20200513\957\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200513\957\1-POS-3MIN.M

Catalog No : HY-130800

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

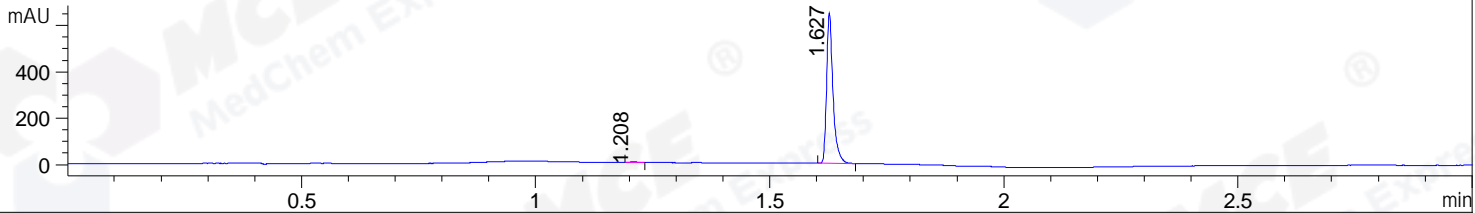


DAD1 C, Sig=254,4 Ref=off

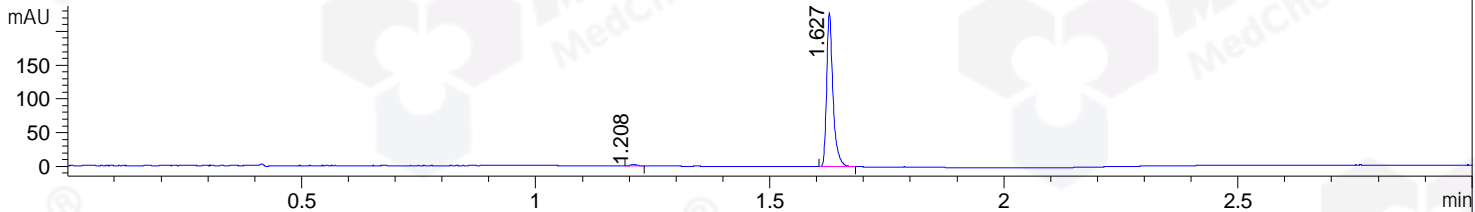

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

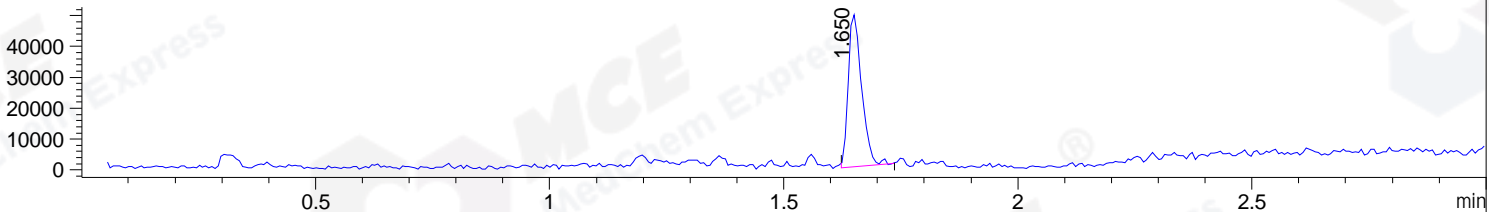

Ion 462, MSD1 462, Target Mass 461 +H Positive, EIC=461.7:462.7

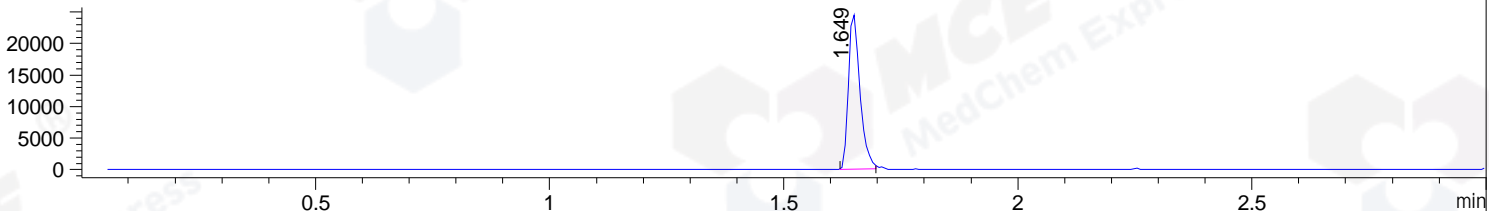

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.02	3.03	3.32	0.49	129
1.63	0.02	612.36	649.74	99.51	462

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.02	1.97	2.02	0.91	129
1.63	0.02	213.62	227.69	99.09	462

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.03	97737.09	49343.64	100.00	462

Ret. Time: 1.65

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

