



File ..TA\2021\20210329\1318\BIZ2021-319-WLQ12-1.D Tgt Mass (CHM) :
 Injection Date : 29 Mar 21 12:53 pm +0800 Seq. Line : 41
 Sample Name : BIZ2021-319-WLQ12-1 Location : P1-F-01
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 5 ul
 Acq. Method : D:\Chem32\1\data\2021\20210329\1318\1-POS-7MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210329\1318\1-POS-7MIN.M
 CAS NO. : 2579696-72-1
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 5 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

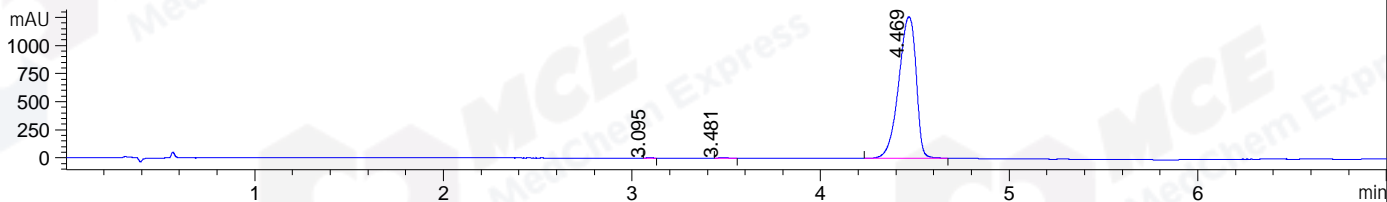


DAD1 C, Sig=254,4 Ref=off

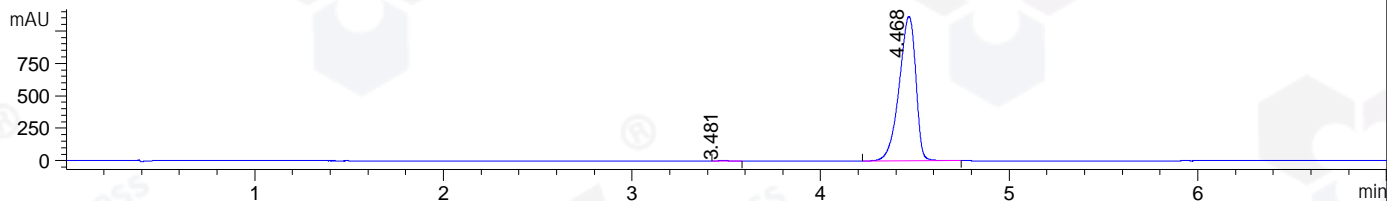

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

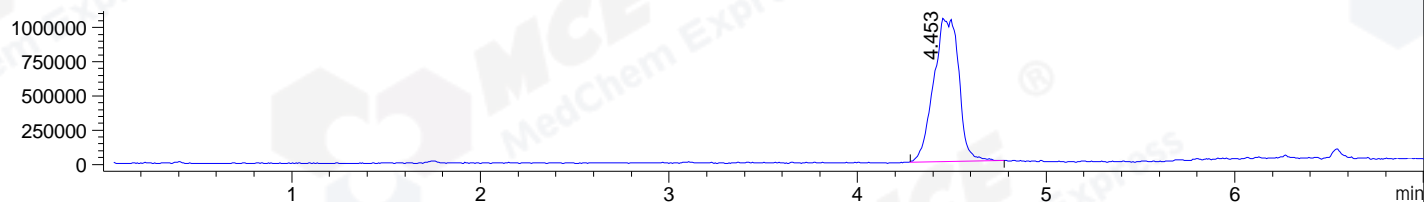

Ion 273, MSD1 273, Target Mass 272 +H Positive, EIC=272.7:273.7

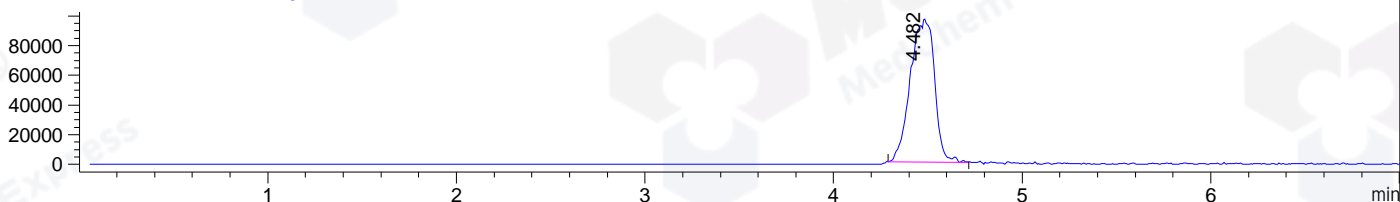

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
3.10	0.03	8.20	4.58	0.10	242
3.48	0.05	13.31	4.69	0.16	ND
4.47	0.11	8084.12	1260.15	99.73	272

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
3.48	0.05	10.89	3.47	0.16	ND
4.47	0.10	6813.86	1114.54	99.84	272

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
4.45	0.15	9765962.00	1054124.25	100.00	272

Ret. Time: 4.45

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

