

File ..DATA\2020\20200730\1058\CPK2020-730-26968.D Tgt Mass (CHM):

Injection Date : 30 Jul 20 4:25 pm +0800 Seq. Line : 89

Sample Name : CPK2020-730-26968 Location : P1-B-09

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200730\1058\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200730\1058\1-POS-3MIN.M

Catalog No : HY-13344

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

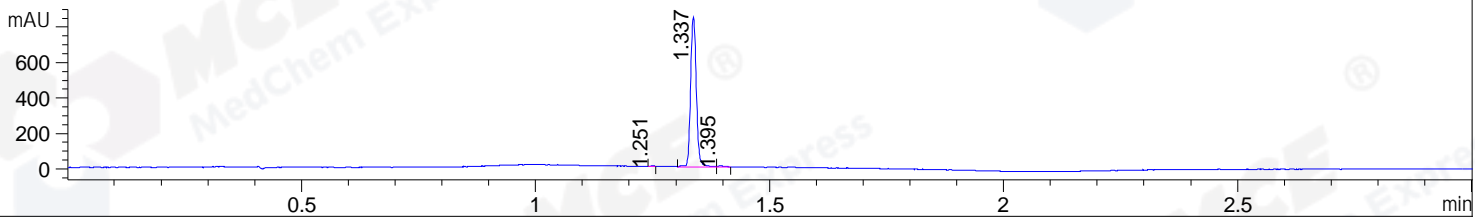


DAD1 C, Sig=254,4 Ref=off

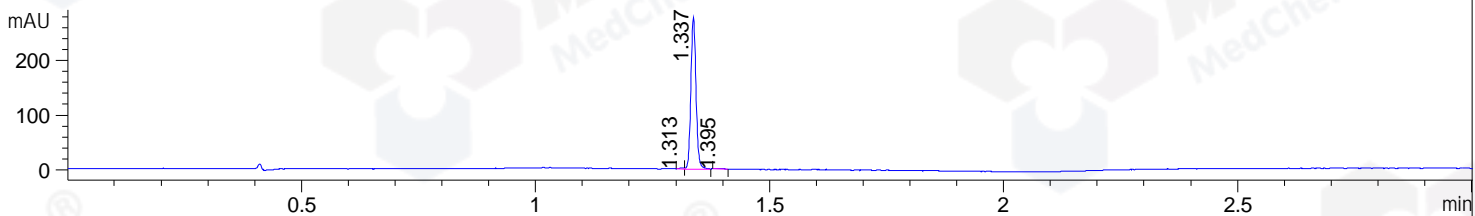

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

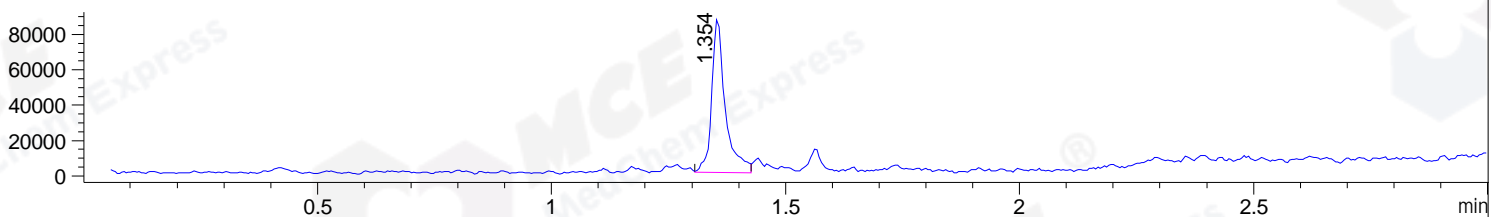

Ion 478, MSD1 478, Target Mass 477 +H Positive, EIC=477.7:478.7

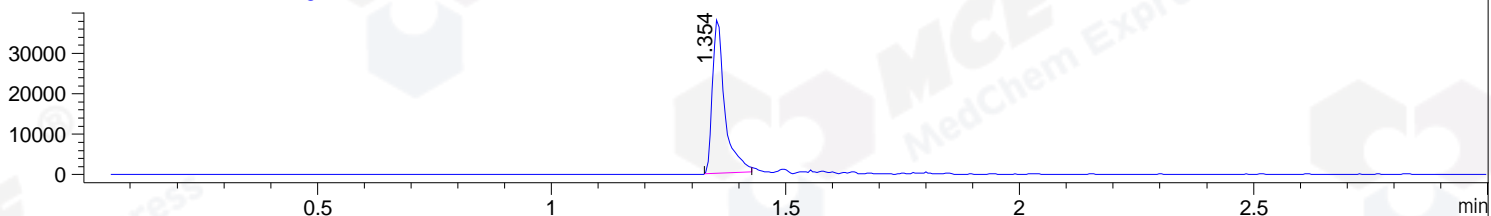

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	1.60	3.42	0.22	645
1.34	0.01	717.98	848.39	99.02	478
1.40	0.02	5.53	6.07	0.76	478

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.31	0.01	1.33	2.03	0.63	ND
1.34	0.01	209.27	278.16	98.95	478
1.40	0.01	0.90	1.19	0.42	478

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.03	176018.16	87241.56	100.00	478

Ret. Time: 1.35

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

