



File ..\DATA\2019\20190423\566\BIZ2019-422-WYQ15.D Tgt Mass (CHM):
 Injection Date : 23 Apr 19 12:16 pm +0800 Seq. Line : 40
 Sample Name : BIZ2019-422-WYQ15 Location : P2-F-08
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190423\566\1-POS-3MIN-1.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190423\566\1-POS-3MIN-1.M
 Catalog No : HY-13418 Batch#40374
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-322
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

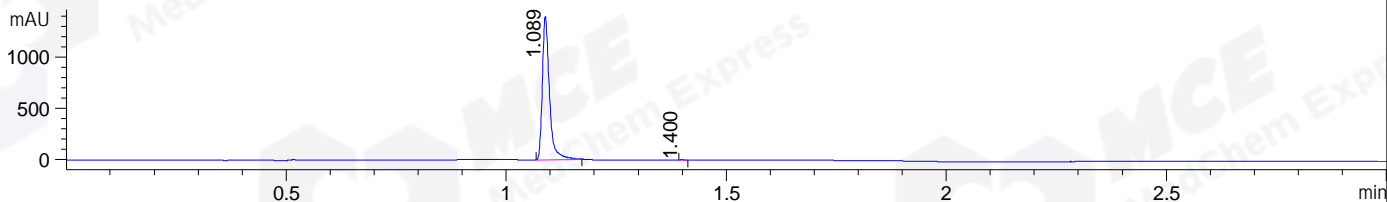


DAD1 C, Sig=254,4 Ref=off

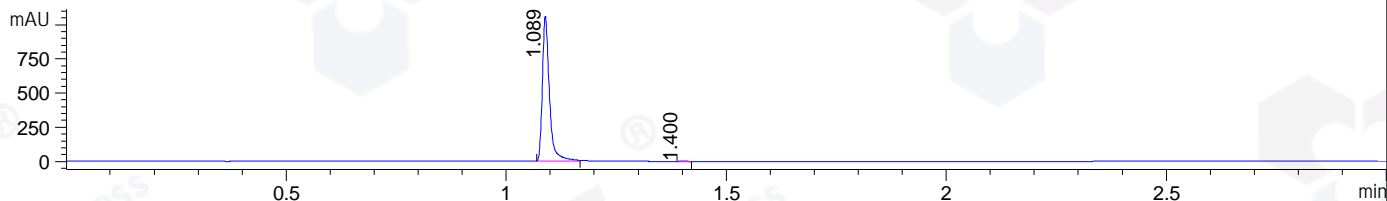

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

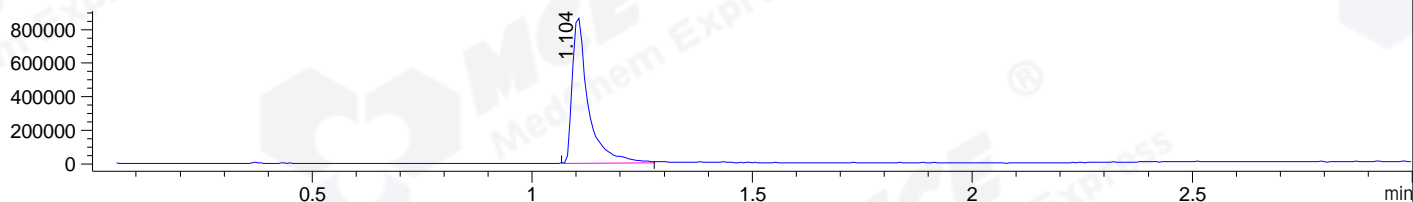

Ion 472.1, MSD1 472.1, Target Mass 471.1 +H Positive, EIC=471.8:472.8

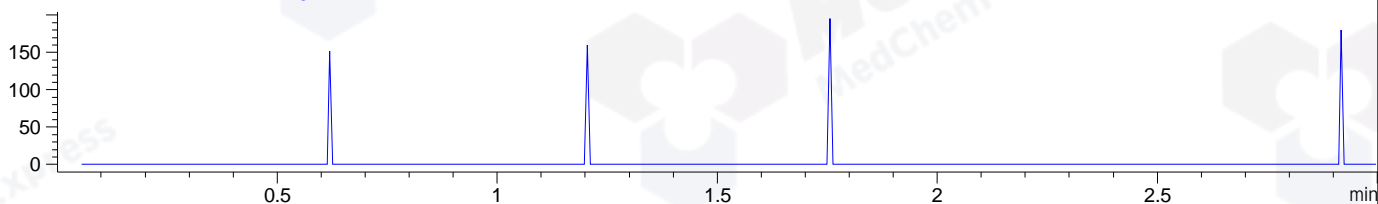

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.02	1584.59	1399.72	99.91	201
1.40	0.01	1.46	2.02	0.09	400

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.02	1186.33	1060.40	99.83	201
1.40	0.02	2.06	2.26	0.17	400

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.04	2192934.50	875510.00	100.00	201

Ret. Time: 1.10

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

