
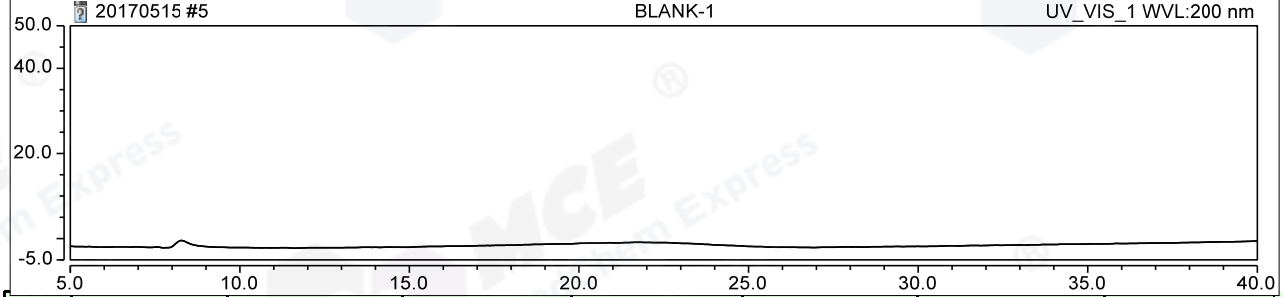


### Chromatogram and Results

#### Injection Details

Injection Name: <b>BLANK-1</b>	Run Time (min): <b>65.00</b>
Vial Number: <b>RA1</b>	Injection Volume: <b>15.00</b>
Injection Type: <b>Unknown</b>	Channel: <b>UV_VIS_1</b>
Instrument: <b>HPLC-17</b>	Wavelength: <b>200</b>
Instrument Method: <b>HY-308_ABC10-H01P54(RP-HPLC)</b>	Dilution Factor: <b>1.0000</b>
Processing Method: <b>Processing Method</b>	Acq. Operator: <b>wkc</b>
Injection Date/Time: <b>15/May/17 19:35</b>	
Comment: <b>A-RP-221(Pro)</b>	

chrom://hy157/XVault/HPLC-17/91/20170515.seq/422.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

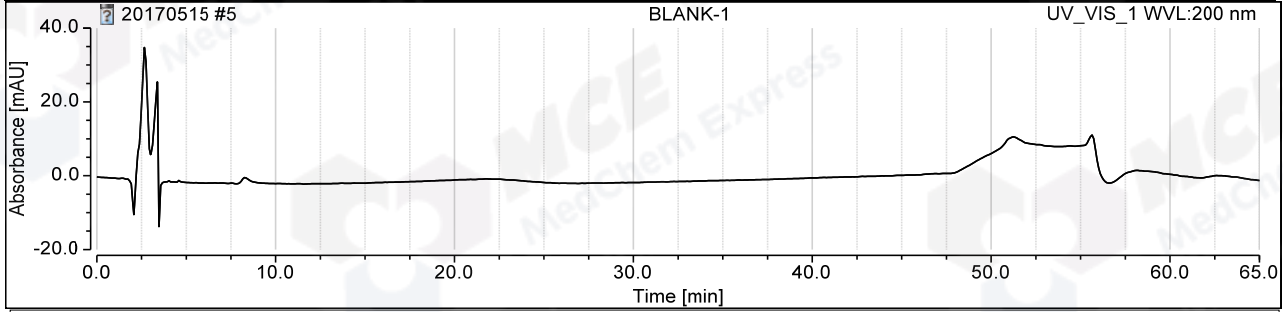



No.	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Plates (EP)	Asymmetry (EP)	Rel.Area %	Peak Name
<b>Total:</b>		<b>0.000</b>	<b>0.000</b>	<b>0.00</b>	<b>0.00</b>			

### Chromatogram and Results

#### Injection Details

Injection Name:	Catalog No: HY-13442A Batch#24757	Run Time (min):	65.00
Vial Number:	RA3	Injection Volume:	15.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Instrument:	HPLC-17	Wavelength:	200
Instrument Method:	HY-308_ABC10-H01P54(RP-HPLC)	Dilution Factor:	1.0000
Processing Method:	Processing Method	Acq. Operator:	wkc
Injection Date/Time:	15/May/17 21:47		
Comment:	A-RP-221(Pro)		

chrom://hy157/XVault/HPLC-17/91/20170515.seq/127.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

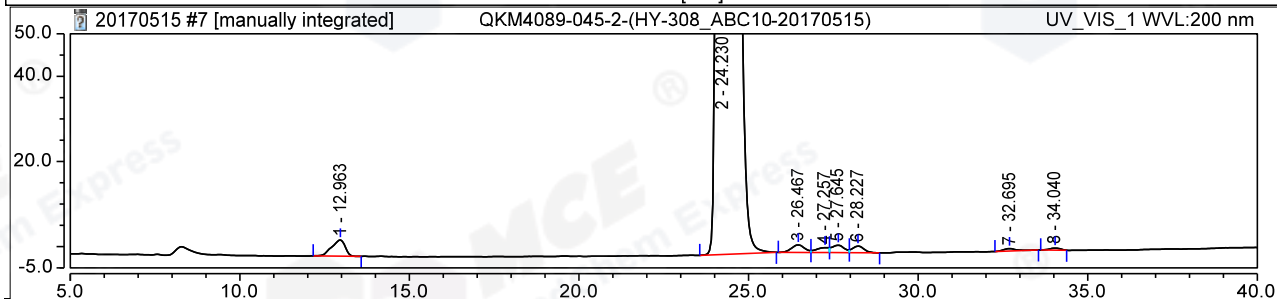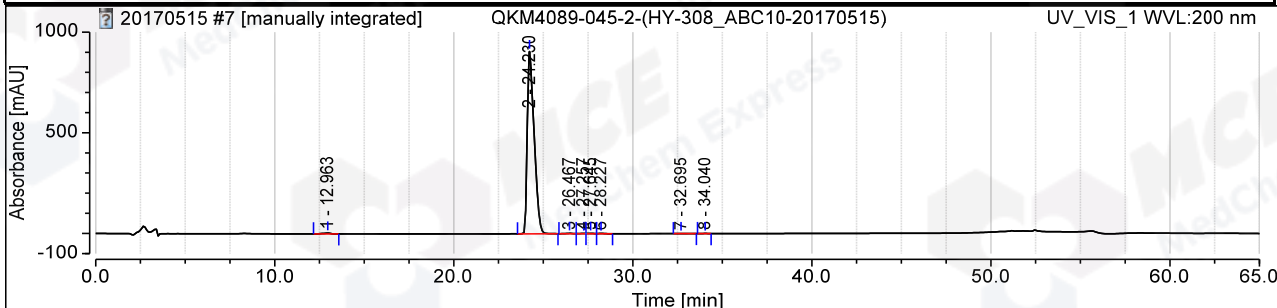

No.	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Plates (EP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	12.963	1.725	3.786	15.16	4547	0.79	0.43	
2	24.230	400.542	905.379	3.13	18038	1.76	98.83	
3	26.467	0.791	1.770	n.a.	22095	n.a.	0.20	
4	27.257	0.484	1.148	n.a.	n.a.	n.a.	0.12	
5	27.645	0.741	1.743	n.a.	n.a.	n.a.	0.18	
6	28.227	0.606	1.546	6.82	27734	n.a.	0.15	
7	32.695	0.231	0.568	2.18	42420	1.15	0.06	
8	34.040	0.165	0.462	n.a.	51003	0.97	0.04	
Total:		405.285	916.402	27.29	165837.00			