
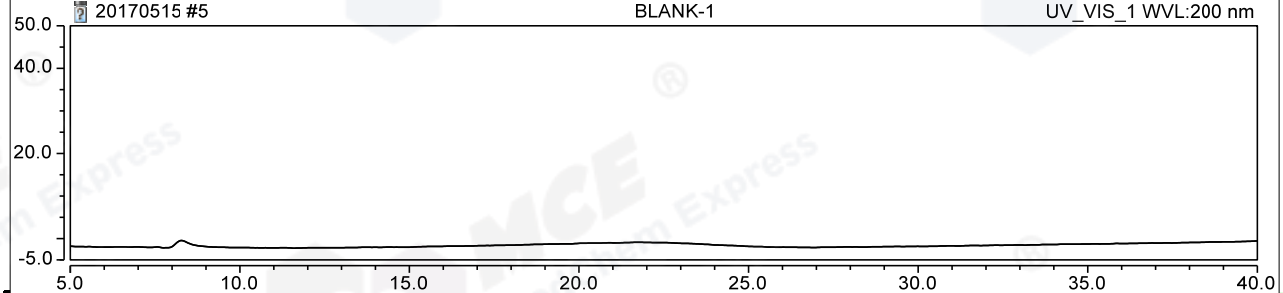


Chromatogram and Results

Injection Details

Injection Name: BLANK-1	Run Time (min): 65.00
Vial Number: RA1	Injection Volume: 15.00
Injection Type: Unknown	Channel: UV_VIS_1
Instrument: HPLC-17	Wavelength: 200
Instrument Method: HY-308_ABC10-H01P54(RP-HPLC)	Dilution Factor: 1.0000
Processing Method: Processing Method	Acq. Operator: wkc
Injection Date/Time: 15/May/17 19:35	
Comment: A-RP-221(Pro)	

chrom://hy157/XVault/HPLC-17/91/20170515.seq/422.smp/UV_VIS_1.channel/UV_VIS_1.chm

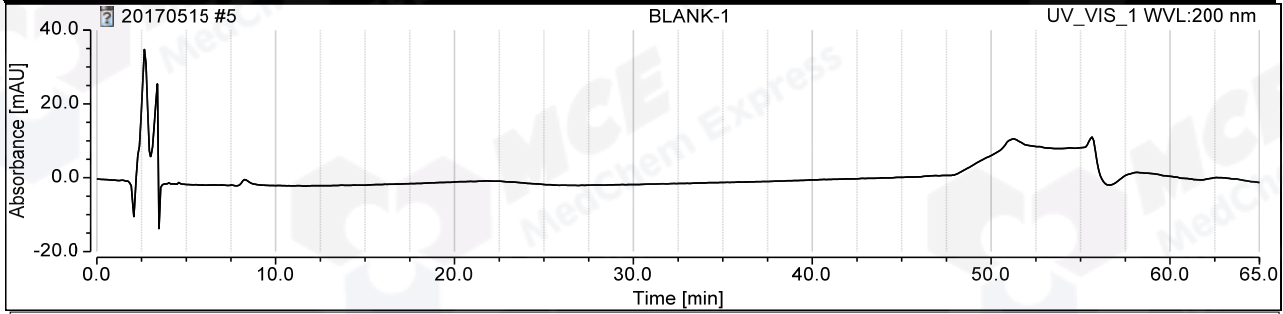



No.	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Plates (EP)	Asymmetry (EP)	Rel.Area %	Peak Name
Total:		0.000	0.000	0.00	0.00			

Chromatogram and Results

Injection Details

Injection Name:	Catalog No: HY-13442A Batch#24757	Run Time (min): 65.00
Vial Number:	RA3	Injection Volume: 15.00
Injection Type:	Unknown	Channel: UV_VIS_1
Instrument:	HPLC-17	Wavelength: 200
Instrument Method:	HY-308_ABC10-H01P54(RP-HPLC)	Dilution Factor: 1.0000
Processing Method:	Processing Method	Acq. Operator: wkc
Injection Date/Time:	15/May/17 21:47	
Comment:	A-RP-221(Pro)	

chrom://hy157/XVault/HPLC-17/91/20170515.seq/127.smp/UV_VIS_1.channel/UV_VIS_1.chm

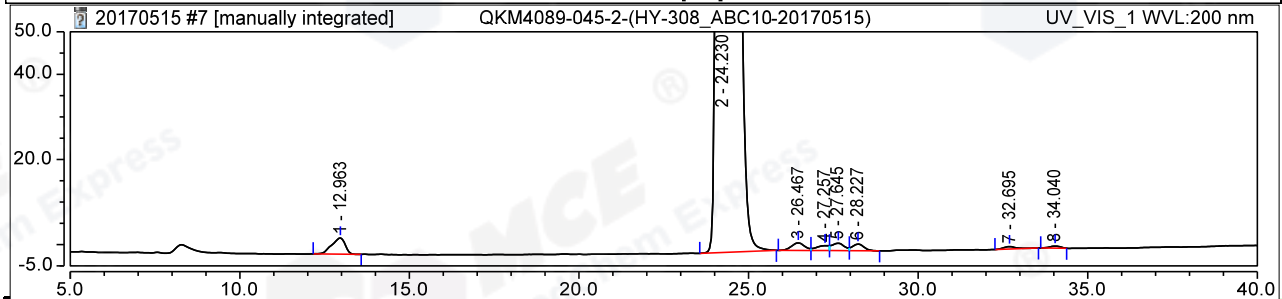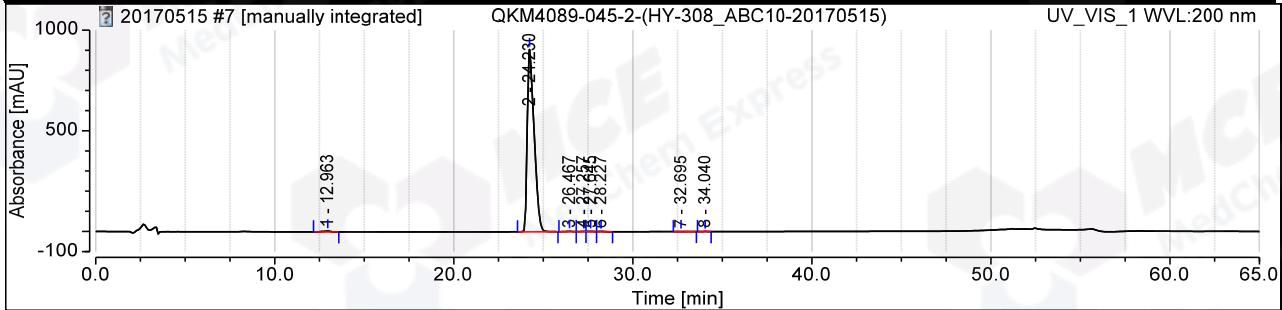

No.	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Plates (EP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	12.963	1.725	3.786	15.16	4547	0.79	0.43	
2	24.230	400.542	905.379	3.13	18038	1.76	98.83	
3	26.467	0.791	1.770	n.a.	22095	n.a.	0.20	
4	27.257	0.484	1.148	n.a.	n.a.	n.a.	0.12	
5	27.645	0.741	1.743	n.a.	n.a.	n.a.	0.18	
6	28.227	0.606	1.546	6.82	27734	n.a.	0.15	
7	32.695	0.231	0.568	2.18	42420	1.15	0.06	
8	34.040	0.165	0.462	n.a.	51003	0.97	0.04	
Total:		405.285	916.402	27.29	165837.00			