



File ..DATA\2020\20200110\810\CPK2020-109-11793-.D Tgt Mass (CHM):
Injection Date : 10 Jan 20 9:04 pm +0800 Seq. Line : 76
Sample Name : CPK2020-109-11793 Location : P1-C-01
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200110\810\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200110\810\1-POS-3MIN.M
Catalog No : HY-13629 Batch# 11793
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

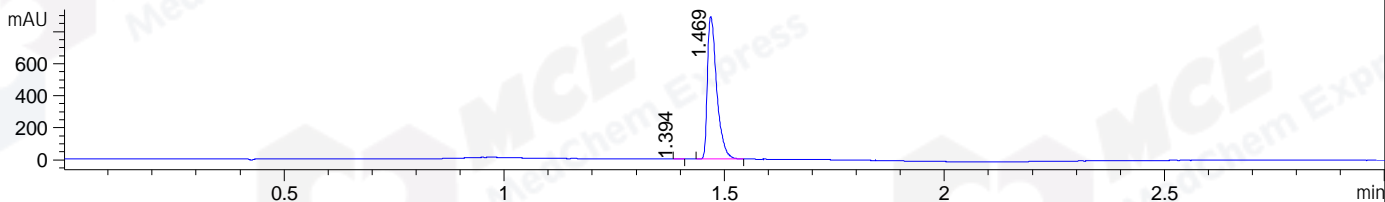


DAD1 C, Sig=254,4 Ref=off

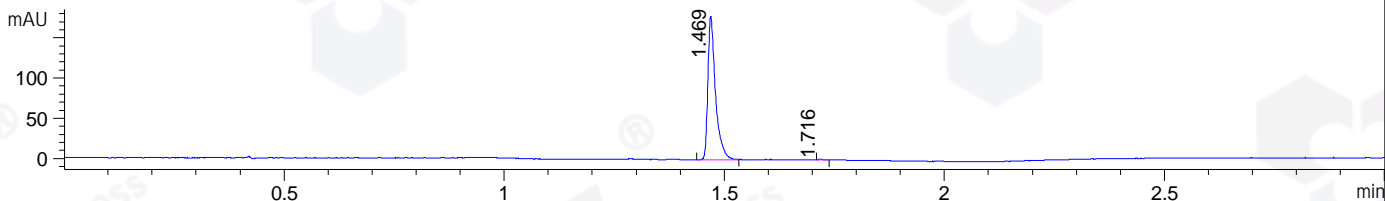

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

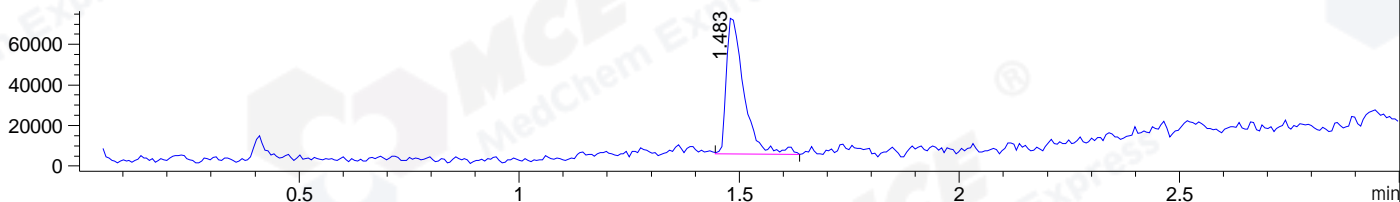

Ion 589, MSD1 589, Target Mass 588 +H Positive, EIC=588.7:589.7

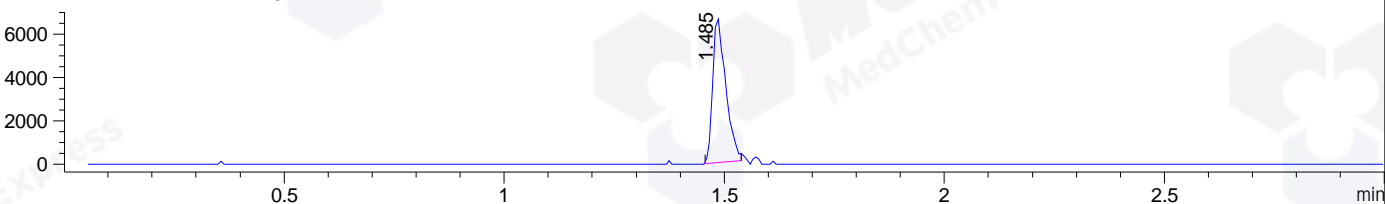

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.39	0.01	0.77	1.09	0.06	ND
1.47	0.02	1316.26	889.98	99.94	606

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.47	0.02	214.75	178.35	99.73	606
1.72	0.01	0.59	0.78	0.27	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.04	184028.00	68792.14	100.00	606

Ret. Time: 1.48

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

