



File ..\DATA\2020\20200928\1119\BIZ2020-927-SCH8.D Tgt Mass (CHM):  
 Injection Date : 28 Sep 20 12:03 pm +0800 Seq. Line : 36  
 Sample Name : BIZ2020-927-SCH8 Location : P1-B-07  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200928\1119\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200928\1119\1-POS-3MIN.M  
 CAS NO. : 135590-91-9  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

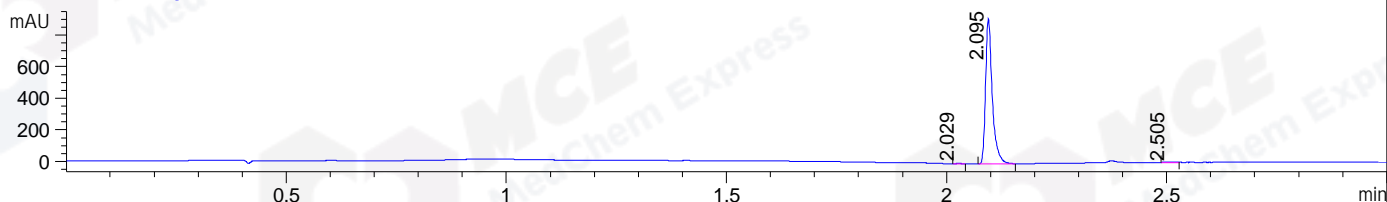


DAD1 C, Sig=254,4 Ref=off

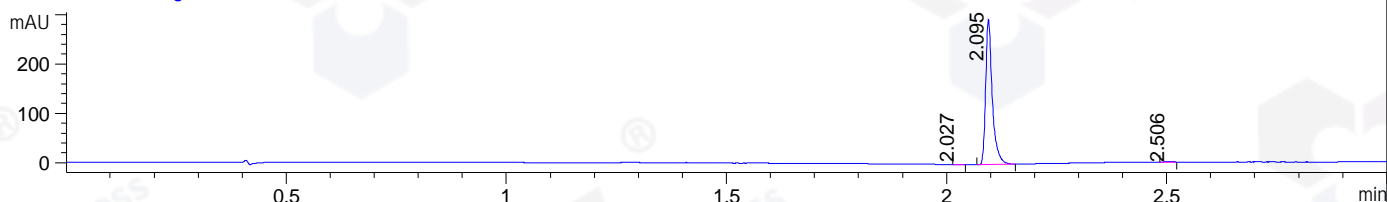

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

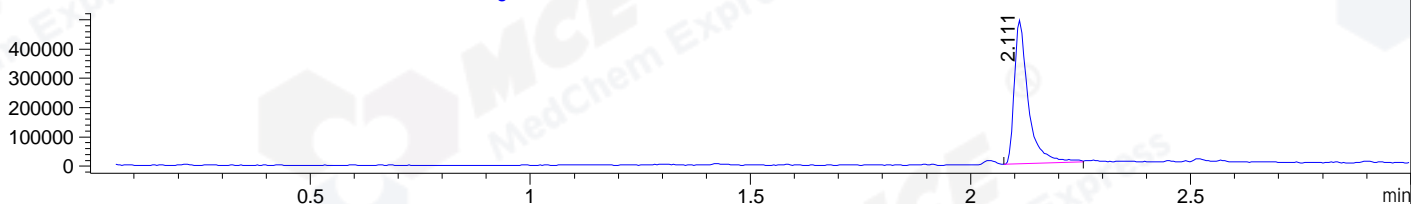

Ion 373, MSD1 373, Target Mass 372 +H Positive, EIC=372.7:373.7

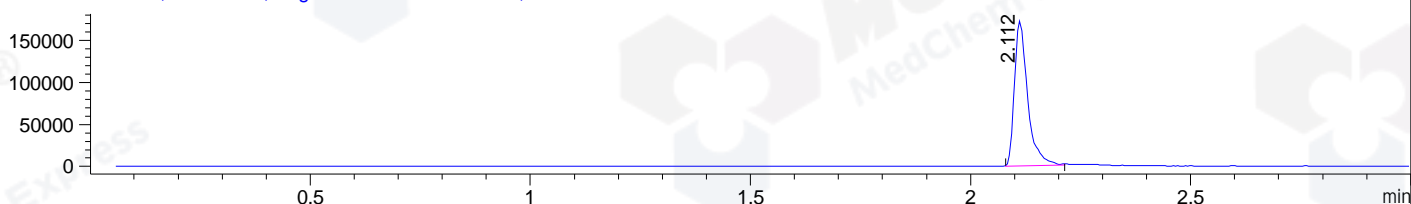

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.03	0.01	1.80	2.02	0.18	359
2.10	0.02	982.32	921.09	99.31	373
2.50	0.02	5.08	4.03	0.51	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.03	0.02	0.62	0.67	0.20	359
2.10	0.02	309.94	294.66	99.32	373
2.51	0.02	1.49	1.27	0.48	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.11	0.03	1092680.75	491810.88	100.00	373

Ret. Time: 2.11

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

