



File ..DATA\2020\20201012\1123\BIZ2020-010-SCH7-.D Tgt Mass (CHM):  
 Injection Date : 12 Oct 20 12:51 pm +0800 Seq. Line : 34  
 Sample Name : BIZ2020-010-SCH7 Location : PL-A-06  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.4 ul  
 Acq. Method : D:\Chem32\1\data\2020\20201012\1123\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20201012\1123\1-POS-3MIN.M  
 Catalog No : HY-136394  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

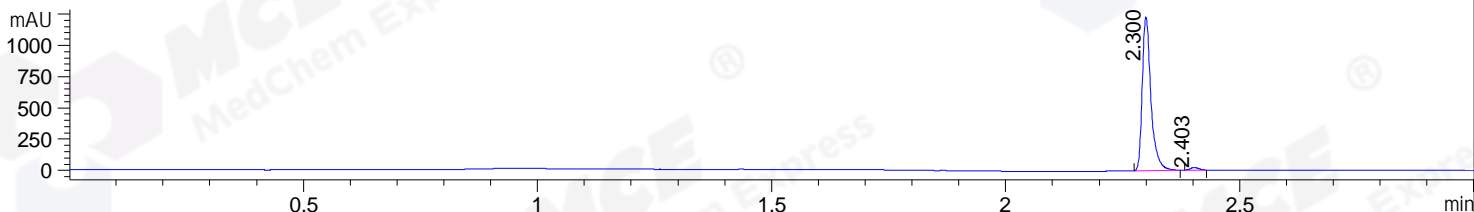


DAD1 C, Sig=254,4 Ref=off

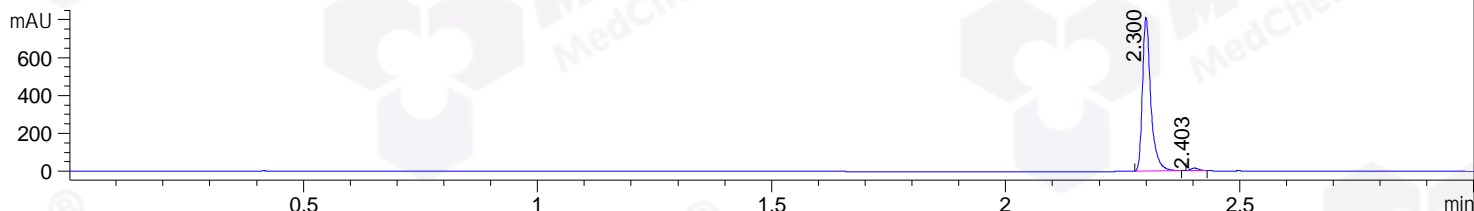

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

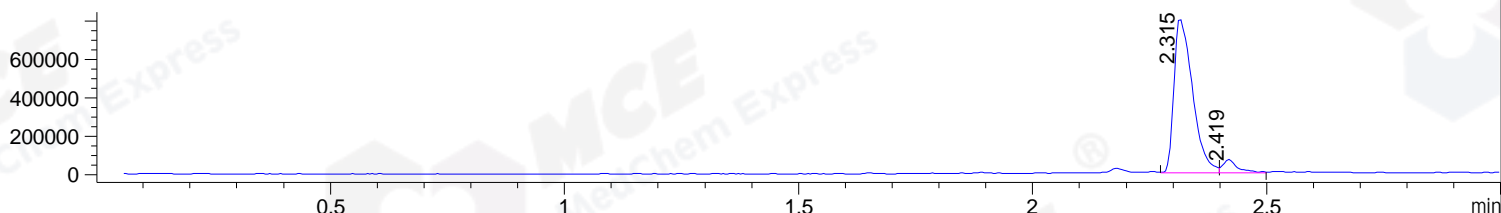

Ion 385, MSD1 385, Target Mass 384 +H Positive, EIC=384.7:385.7

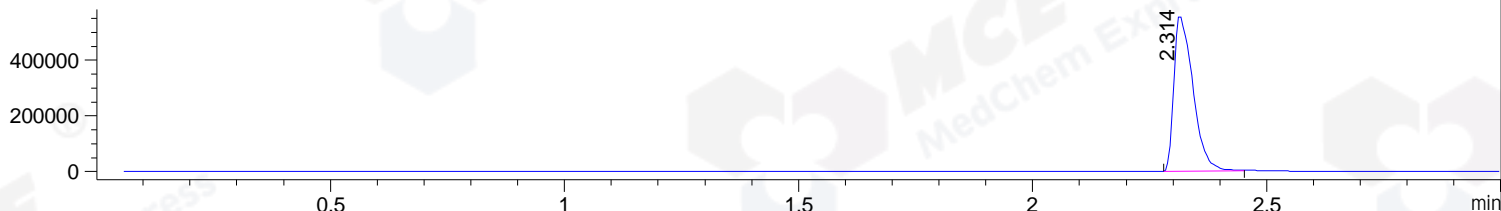

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.30	0.02	1586.58	1229.74	98.37	385
2.40	0.02	26.26	21.55	1.63	385

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.30	0.02	1004.15	811.77	98.46	385
2.40	0.02	15.68	13.03	1.54	385


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.31	0.04	2227923.75	802583.19	93.35	385
2.42	0.03	158691.91	70049.75	6.65	583

Ret. Time: 2.31

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

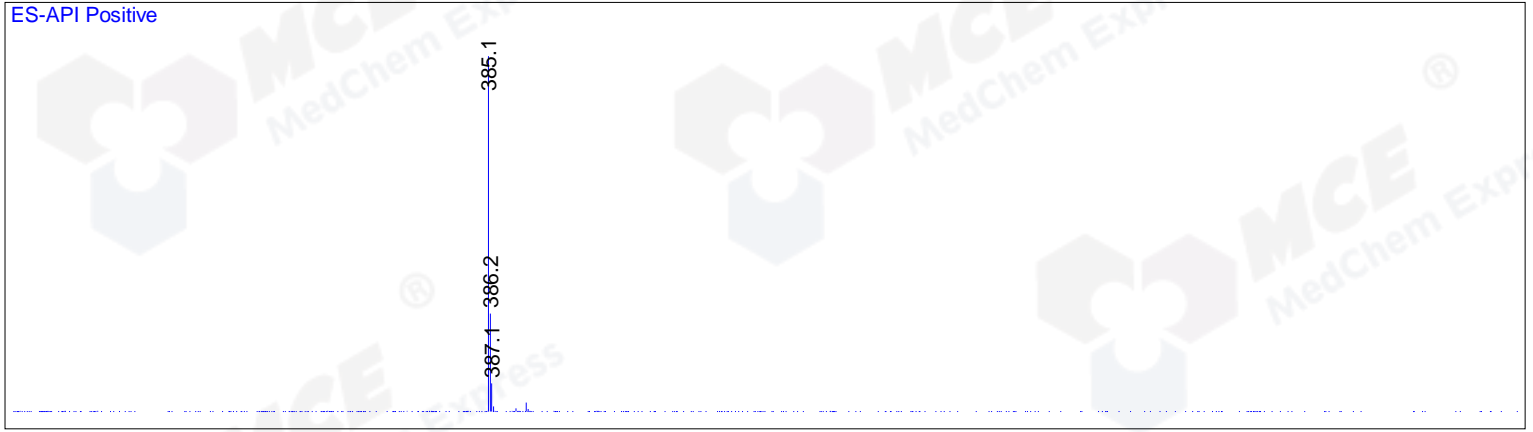

Ret. Time: 2.42

ES-API Positive

